
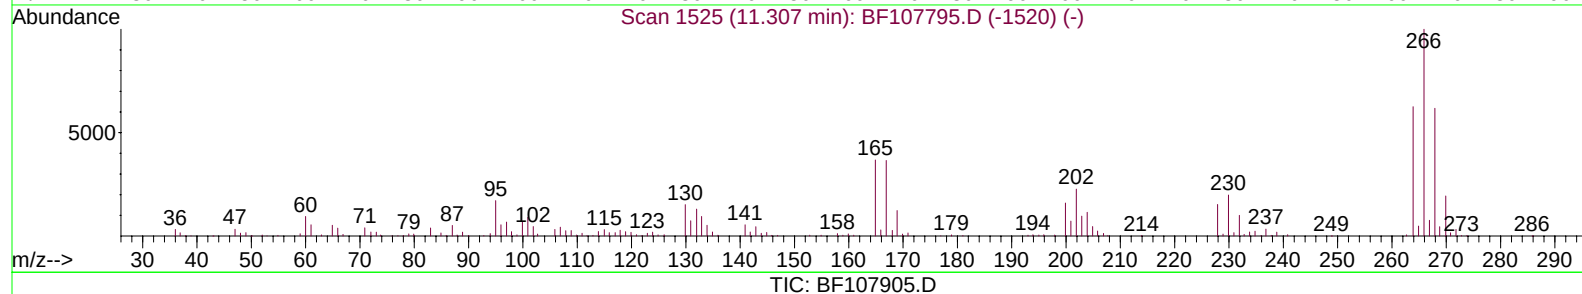
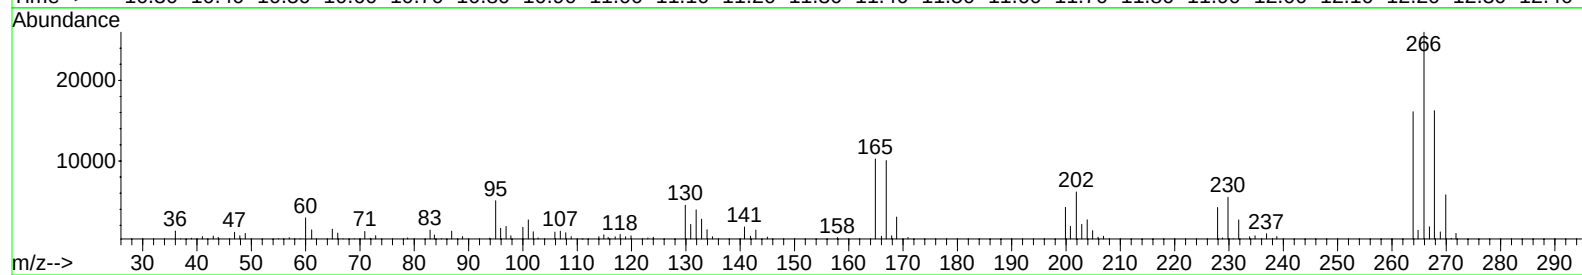


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF080218\
Data File : BF107905.D
Acq On : 2 Aug 2018 13:19
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:30:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 30 17:48:53 2018
Response via : Initial Calibration

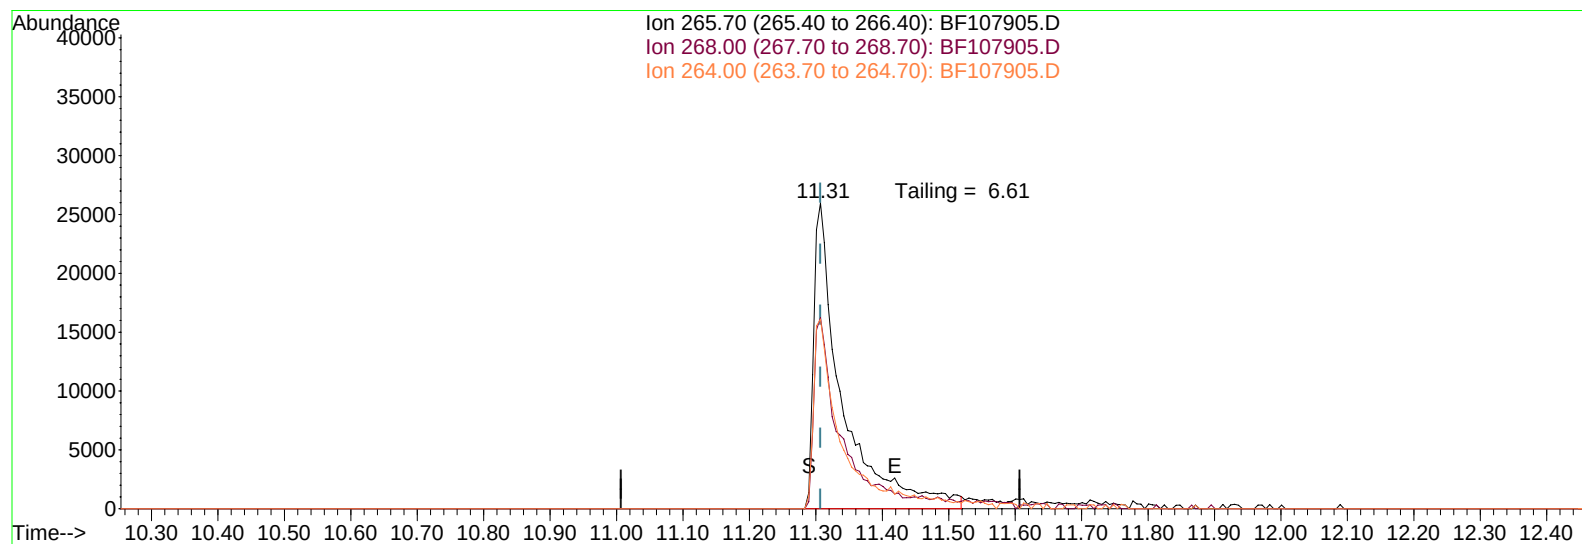

(69) Pentachlorophenol (C)




11.307min (+0.000) 22593.41ng

response 73170

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.51
264.00	61.90	62.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF080218\
 Data File : BF107905.D
 Acq On : 2 Aug 2018 13:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:30:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 30 17:48:53 2018
 Response via : Initial Calibration

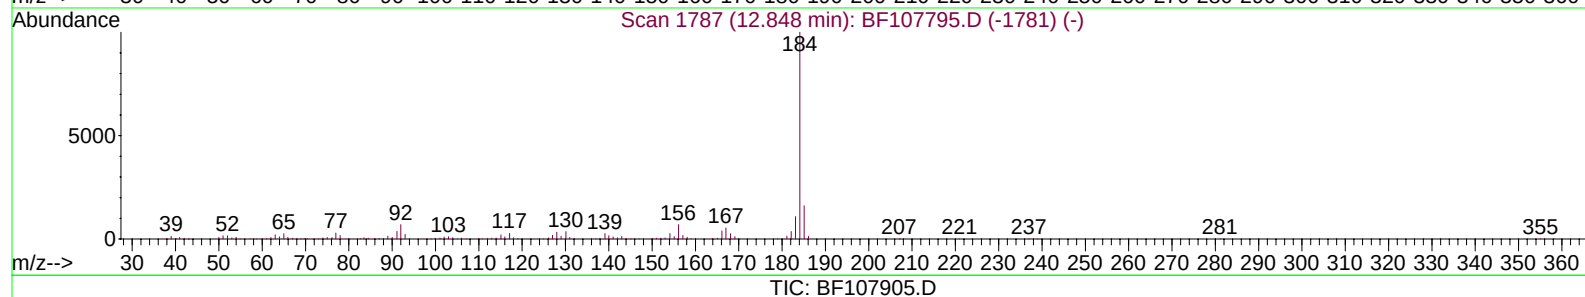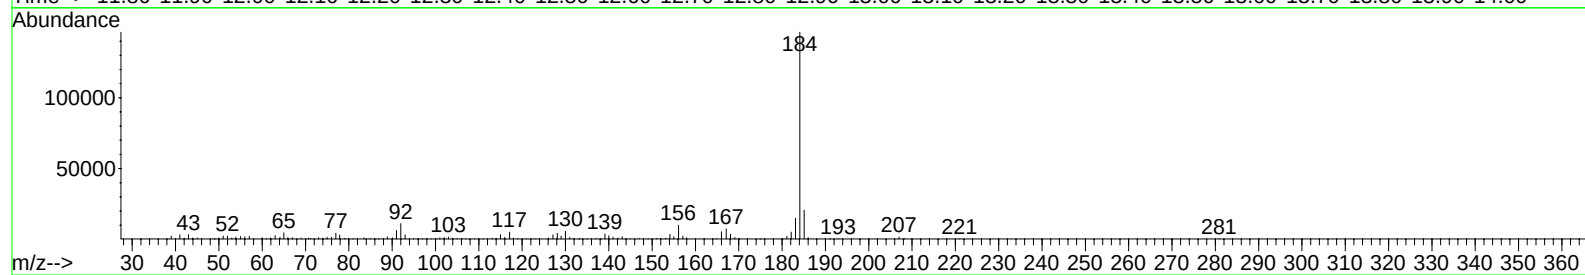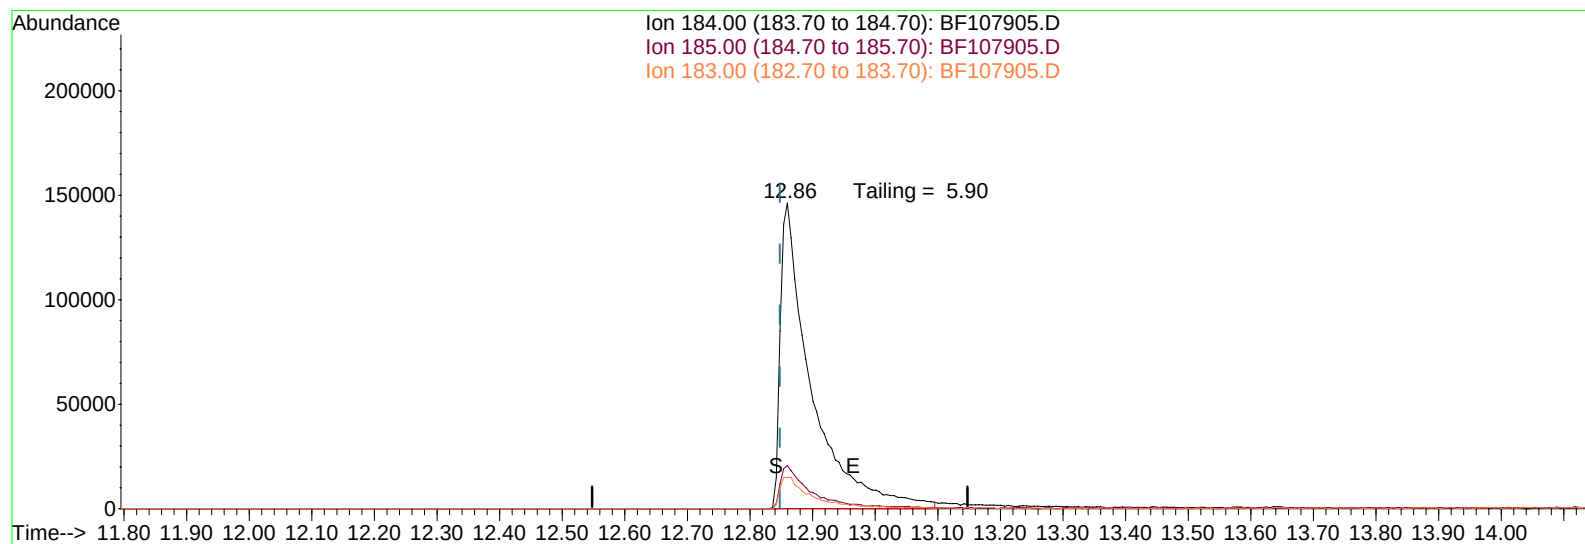

(76) Benzidine

12.860min (+0.012) 117254.28ng

response 508011

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.12
183.00	11.60	10.18
0.00	0.00	0.00