


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080218\
 Data File : BF107931.D
 Acq On : 3 Aug 2018 1:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 30 17:48:53 2018

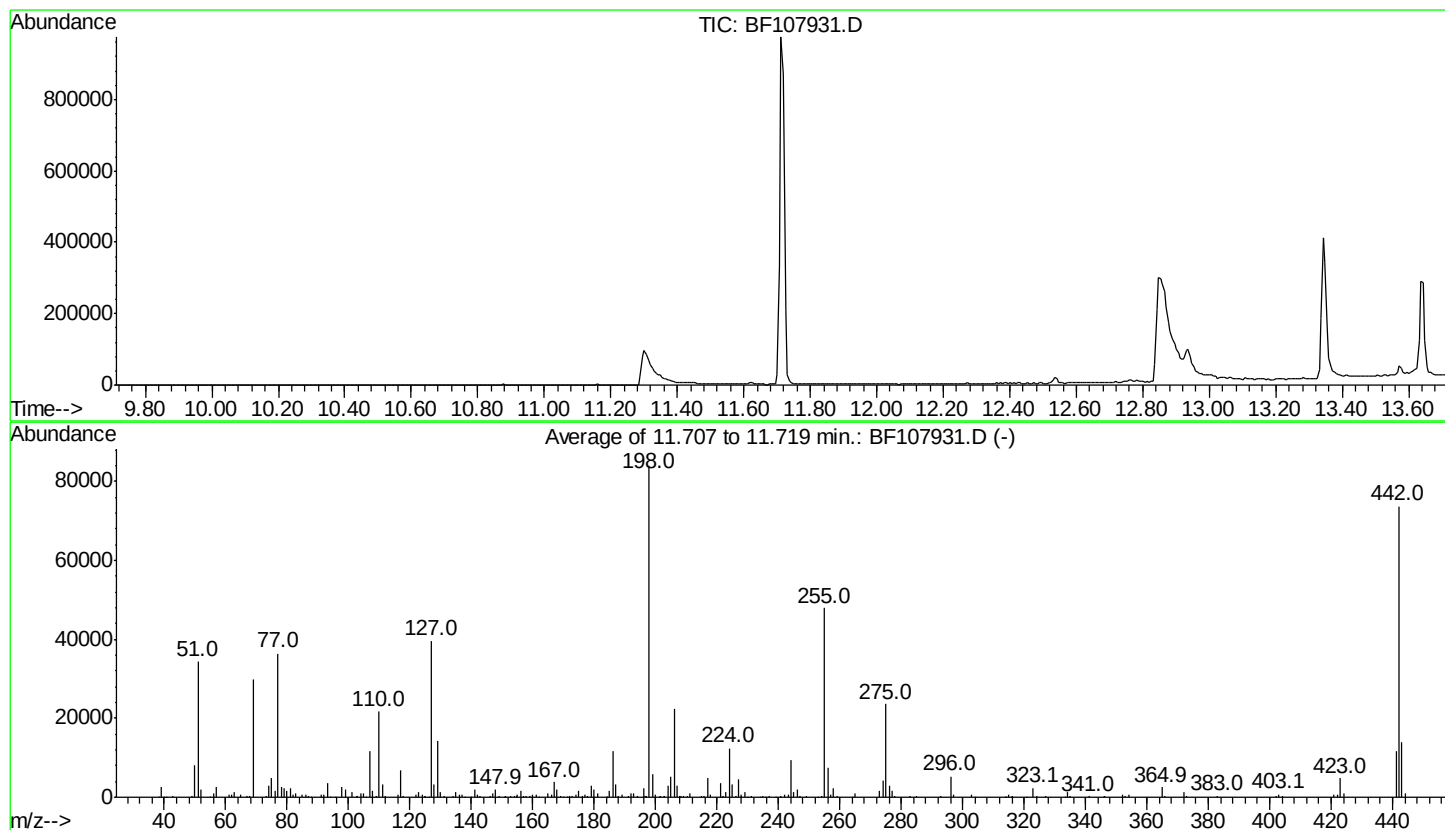

AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	34226	PASS
68	69	0.00	2	1.3	380	PASS
69	198	0.00	100	35.6	29880	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.2	39637	PASS
197	198	0.00	2	0.3	261	PASS
198	198	100	100	100.0	83984	PASS
199	198	5	9	7.0	5858	PASS
275	198	10	60	28.0	23557	PASS
365	198	1	100	3.1	2562	PASS
441	198	0.01	100	14.0	11724	PASS
442	198	50	100	87.8	73697	PASS
443	442	15	24	19.0	13986	PASS