
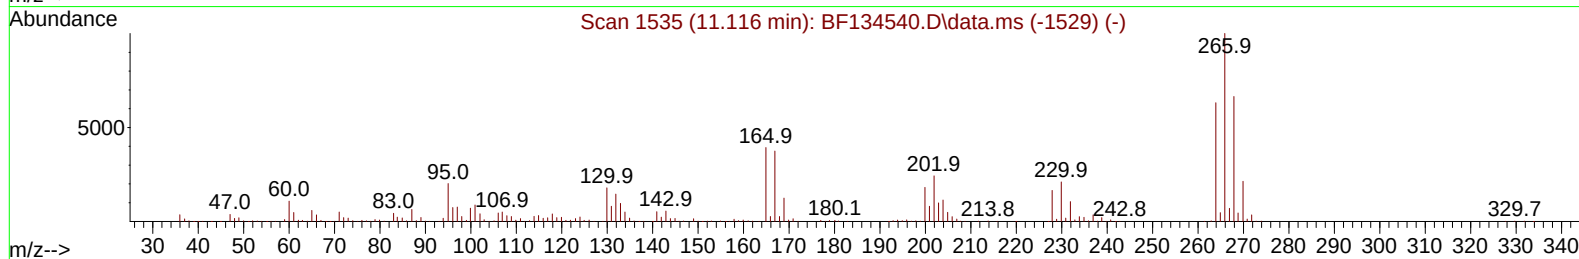
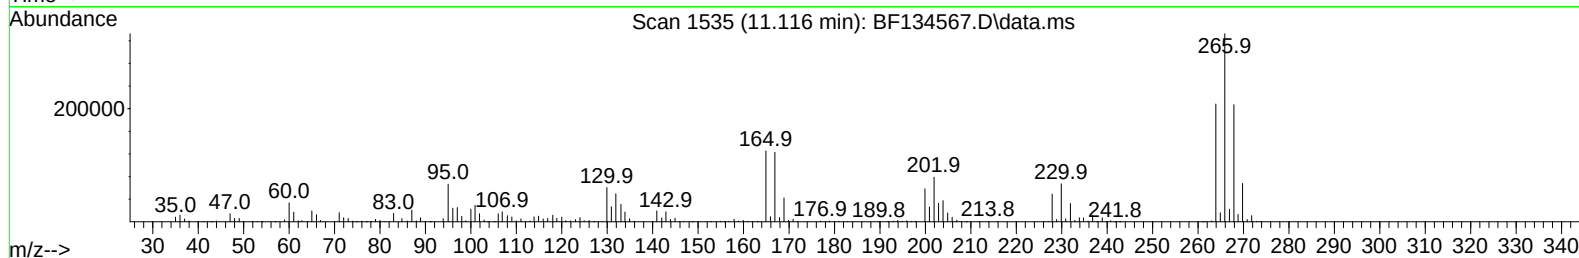


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134567.D
Acq On : 02 Aug 2023 08:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:34:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

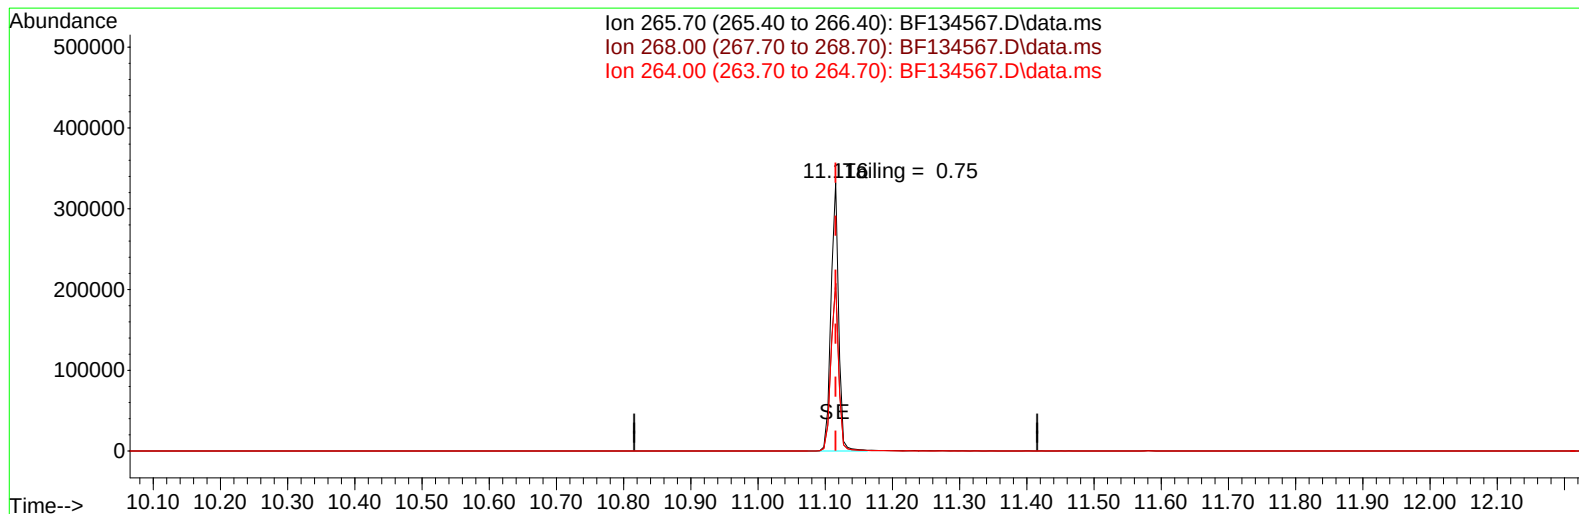

TIC: BF134567.D\data.ms

(70) Pentachlorophenol (C)




11.116min (+ 0.000) 611186.26 ng

response 266843

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.35
264.00	59.70	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134567.D
Acq On : 02 Aug 2023 08:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:34:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

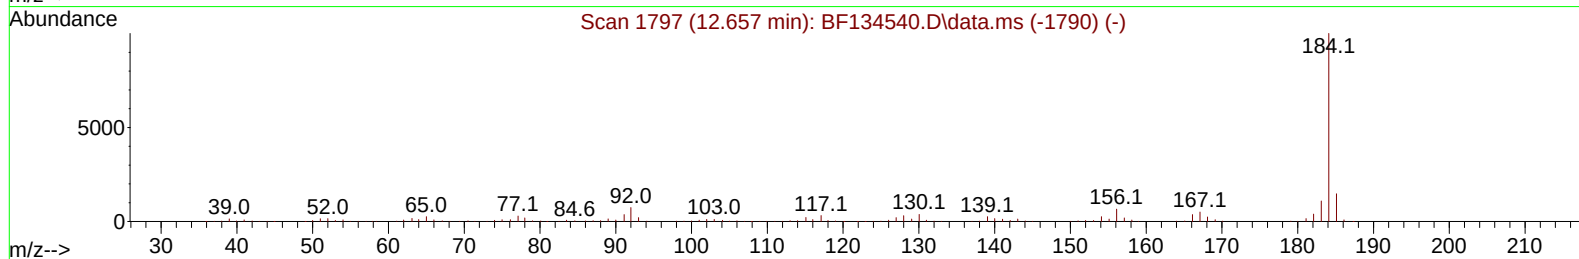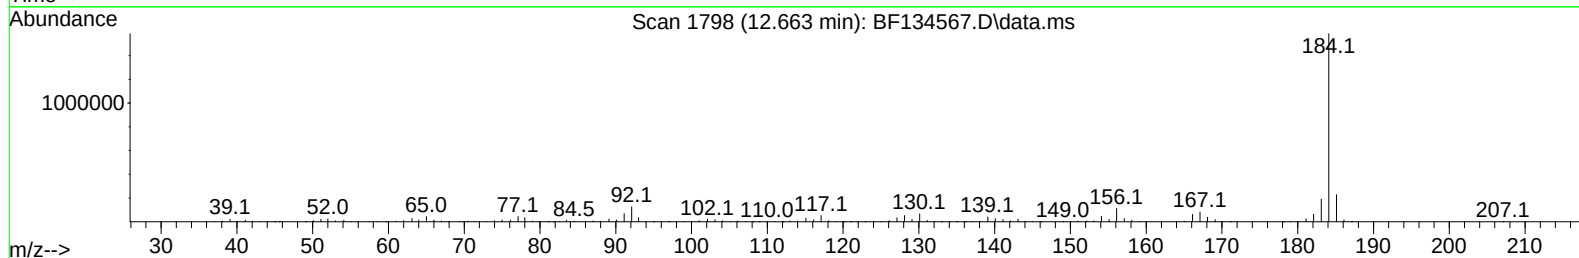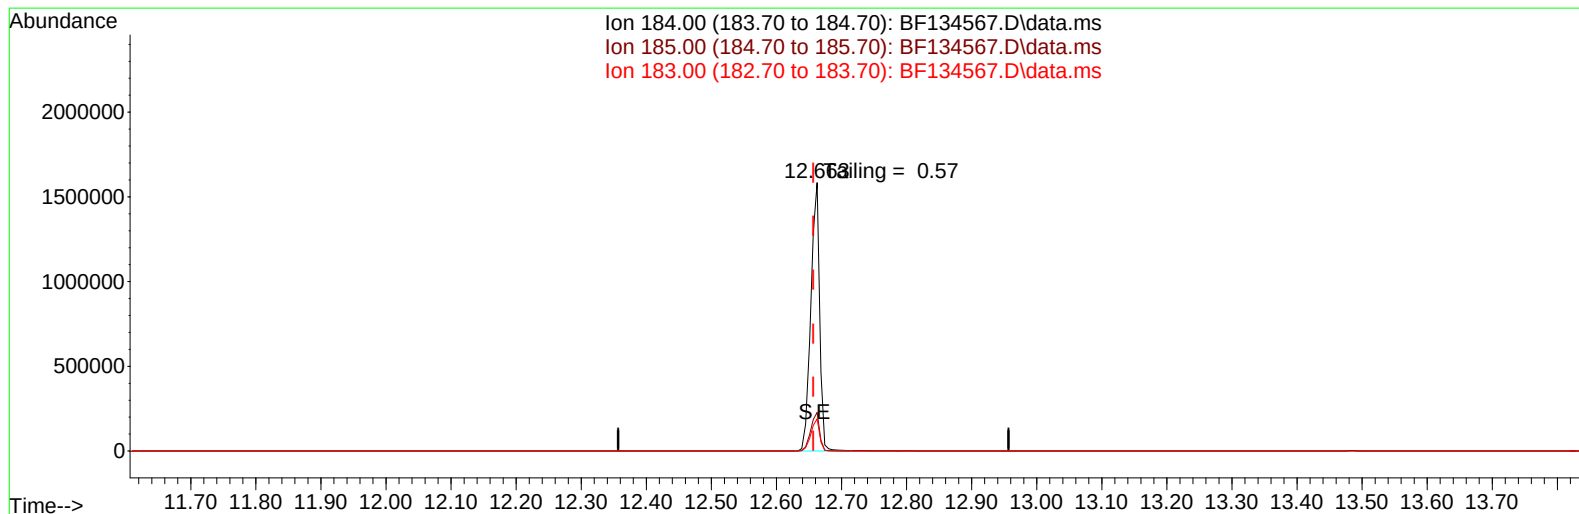

TIC: BF134567.D\data.ms

(77) Benzidine**12.663min (+ 0.006) 623264.74 ng****response 1501803**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.36
183.00	10.80	12.00
0.00	0.00	0.00