
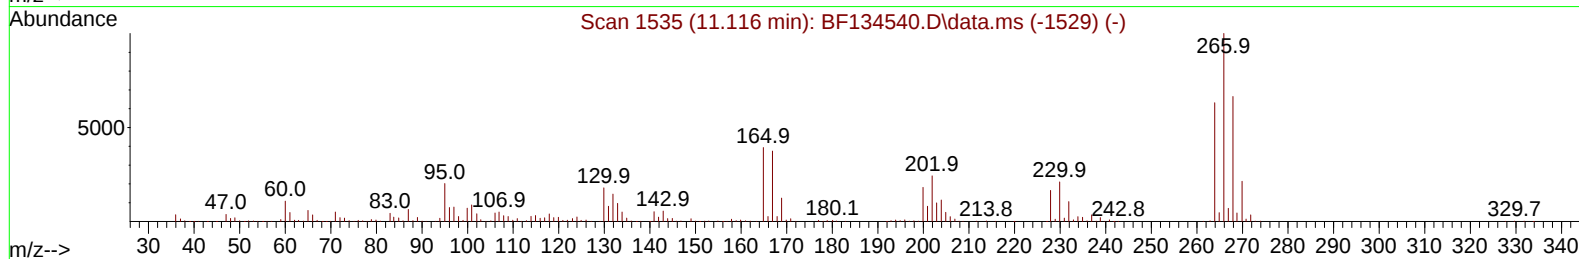
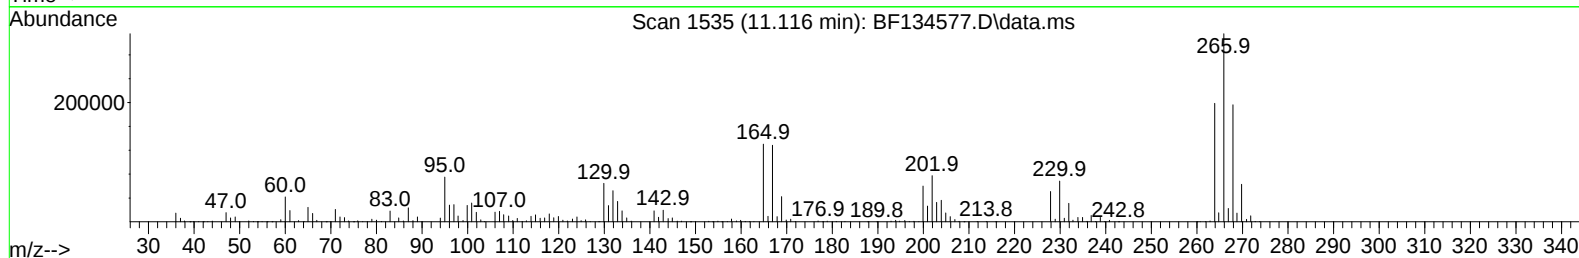


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134577.D
Acq On : 02 Aug 2023 13:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 15:38:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

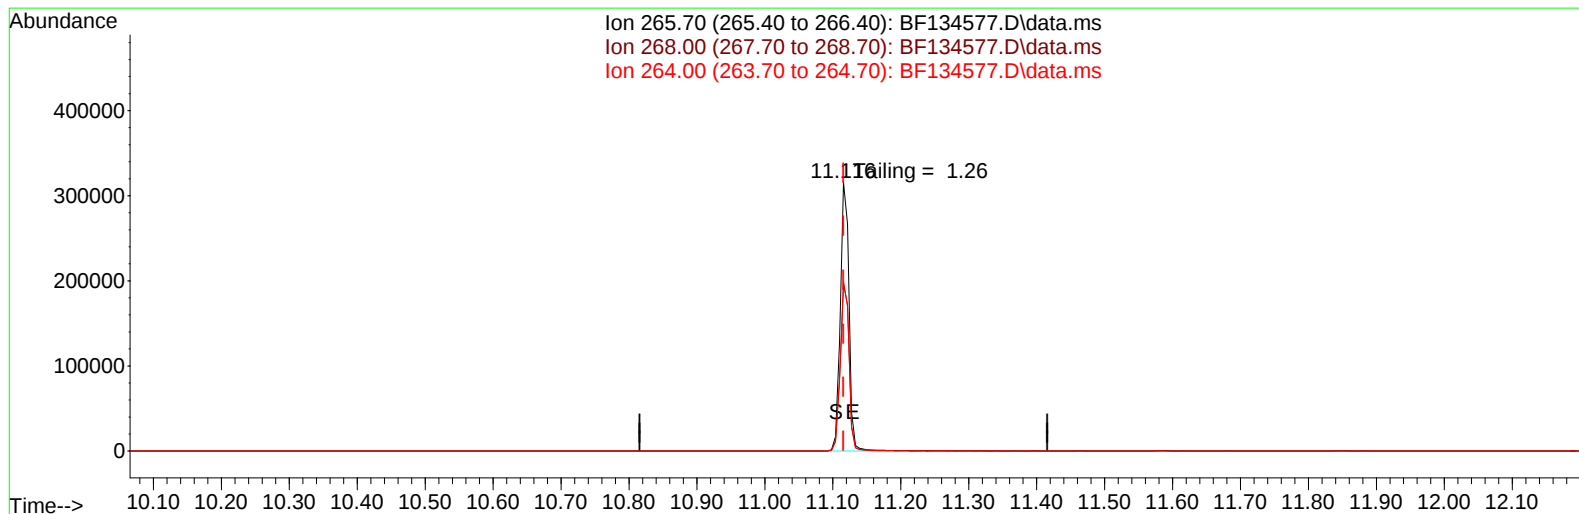

TIC: BF134577.D\data.ms

(70) Pentachlorophenol (C)




11.116min (+ 0.000) 536612.68 ng

response 280373

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.26
264.00	59.70	62.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134577.D
Acq On : 02 Aug 2023 13:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 15:38:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

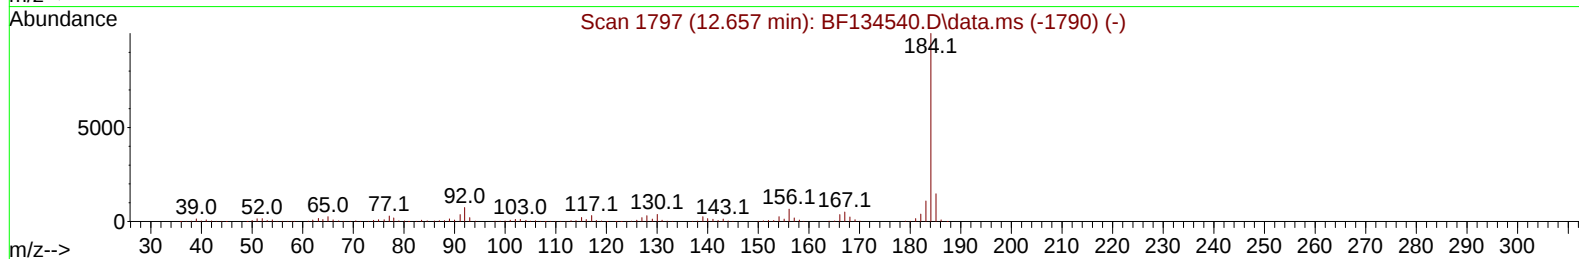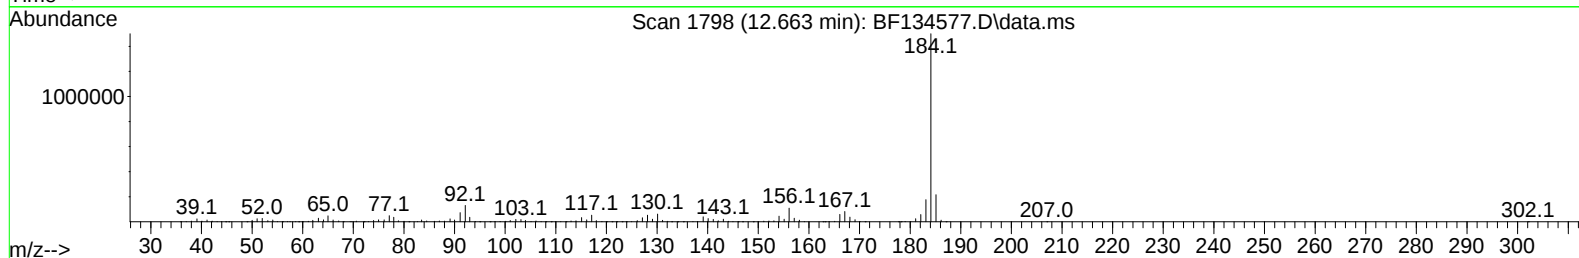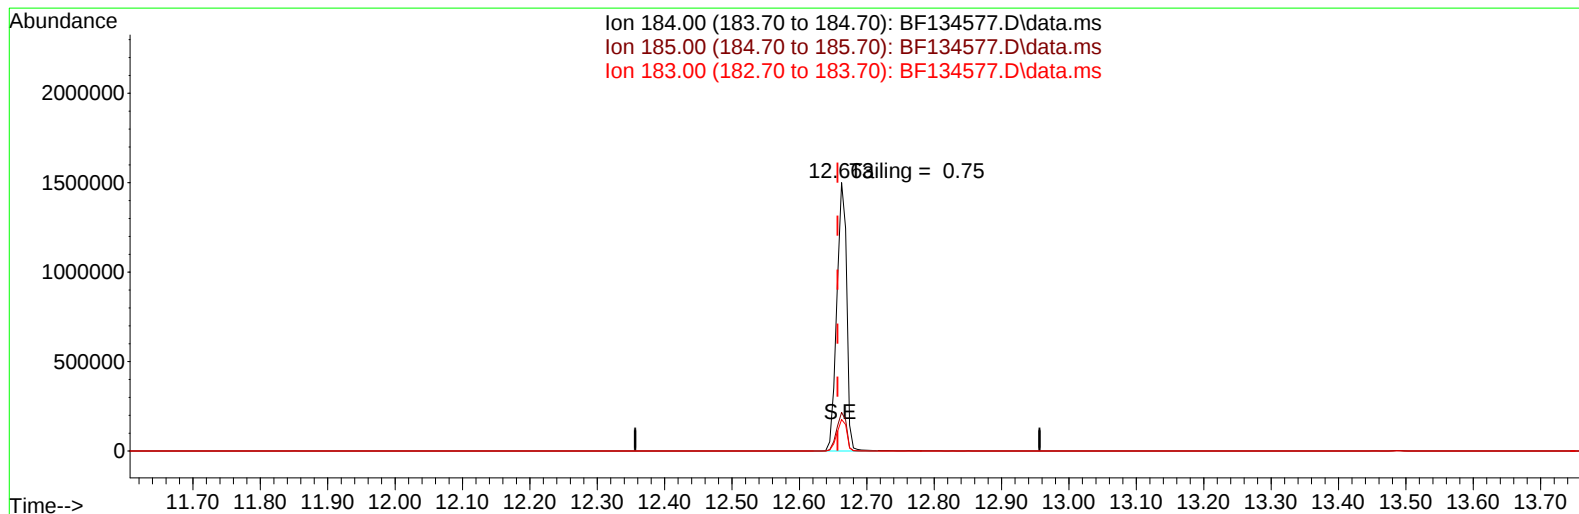

TIC: BF134577.D\data.ms

(77) Benzidine**12.663min (+ 0.006) 240370.22 ng****response 1523635**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.41
183.00	10.80	11.74
0.00	0.00	0.00