

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
 Data File : BF134575.D
 Acq On : 02 Aug 2023 12:26
 Operator : CG\JU
 Sample : 03681-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RPTP-7-CS-7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.857	293	301	308	rVB	27457	42001	1.39%	0.194%
2	5.416	561	566	569	rBV	3284562	3017017	100.00%	13.916%
3	6.422	732	737	740	rBV	3009354	3000652	99.46%	13.841%
4	6.793	797	800	804	rBV	1340172	1191366	39.49%	5.495%
5	7.351	891	895	898	rBV	1922426	1734007	57.47%	7.998%
6	8.075	1014	1018	1021	rBV	1739687	1405286	46.58%	6.482%
7	9.151	1197	1201	1204	rVB	3437546	2716990	90.06%	12.532%
8	9.828	1312	1316	1319	rBV	1536878	1179770	39.10%	5.442%
9	10.610	1446	1449	1453	rBV	1475054	1336814	44.31%	6.166%
10	11.316	1565	1569	1571	rBV	1344389	1129543	37.44%	5.210%
11	11.333	1571	1572	1576	rVV	120361	93275	3.09%	0.430%
12	11.386	1576	1581	1585	rVB	42583	39784	1.32%	0.184%
13	11.851	1656	1660	1664	rBV2	92510	93537	3.10%	0.431%
14	12.527	1771	1775	1779	rBV	239983	197348	6.54%	0.910%
15	12.757	1808	1814	1818	rBV	184692	199282	6.61%	0.919%
16	12.910	1836	1840	1843	rBV	2903567	2510250	83.20%	11.579%
17	13.821	1992	1995	1999	rVB	110756	108493	3.60%	0.500%
18	13.957	2014	2018	2021	rBV	1095454	984422	32.63%	4.541%
19	13.980	2021	2022	2025	rVB	65330	46303	1.53%	0.214%
20	15.421	2263	2267	2271	rBV	564362	653779	21.67%	3.016%




Sum of corrected areas: 21679919

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134575.D
Acq On : 02 Aug 2023 12:26
Operator : CG\JU
Sample : 03681-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RPTP-7-CS-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

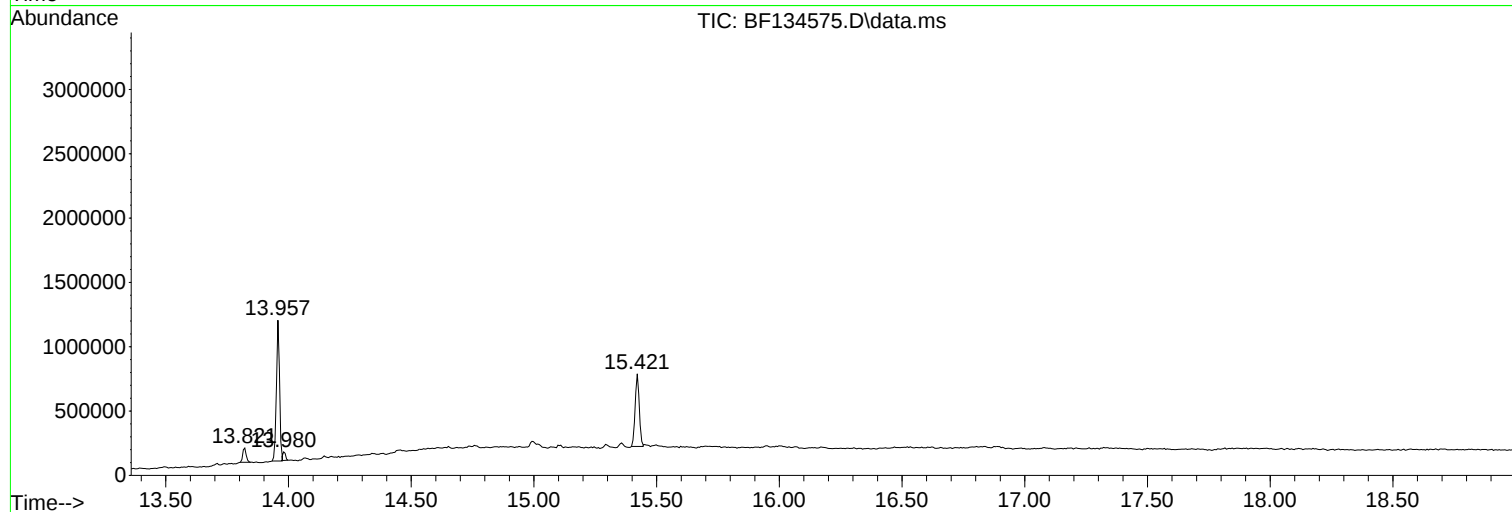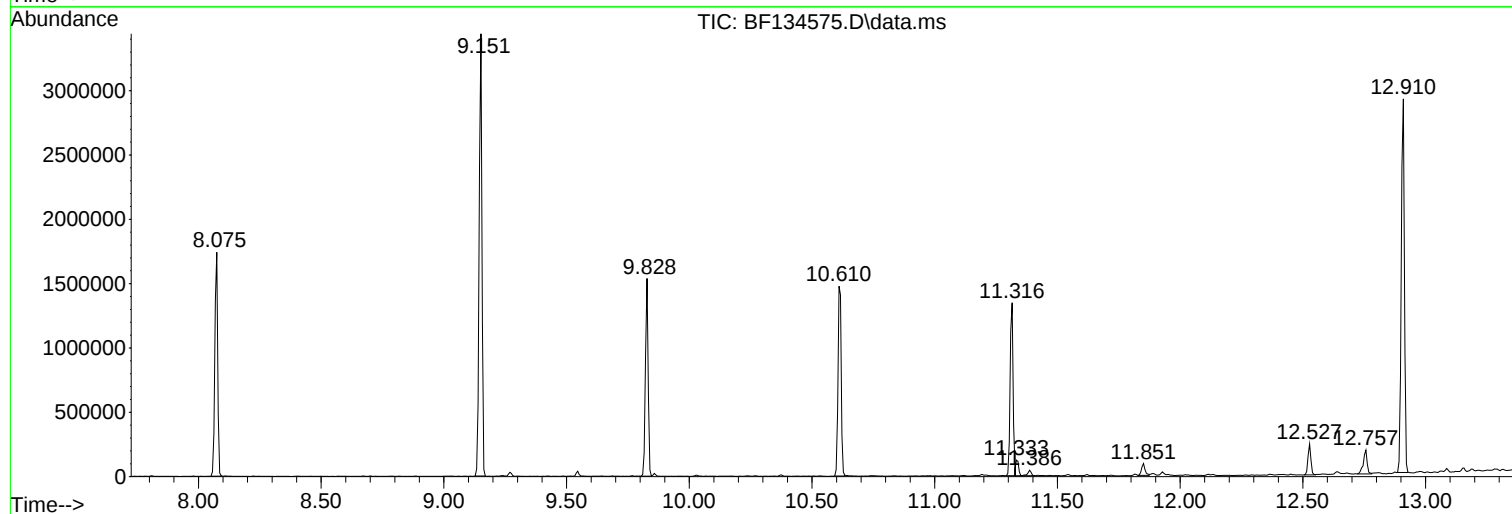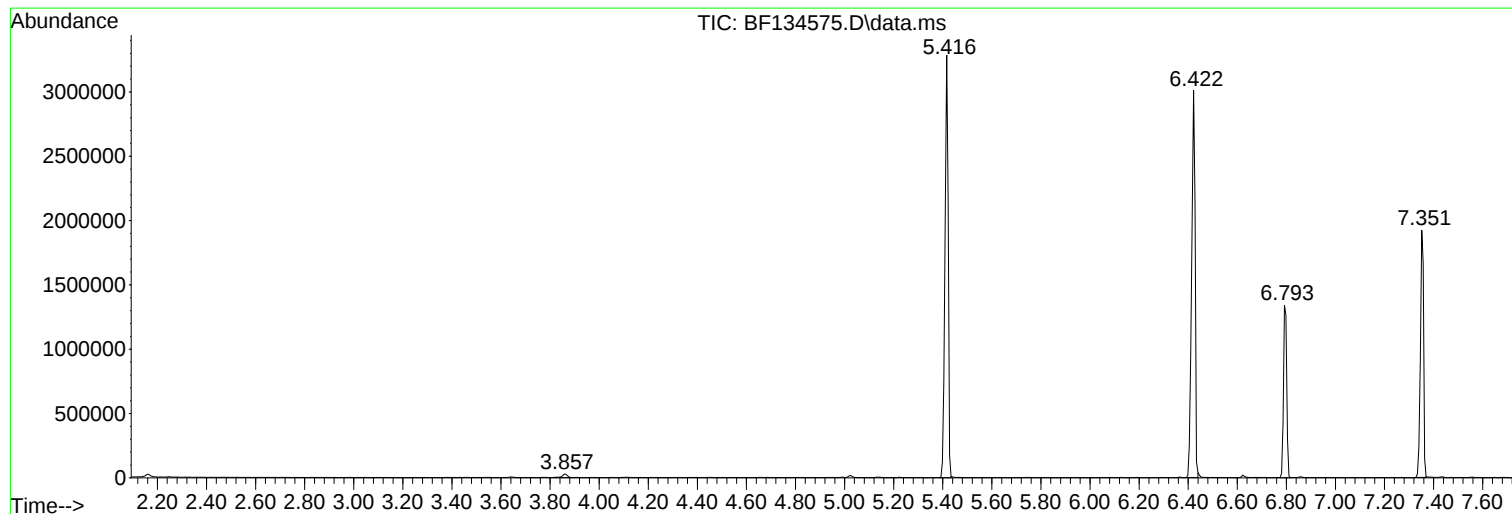

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134575.D
Acq On : 02 Aug 2023 12:26
Operator : CG\JU
Sample : 03681-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RPT-7-CS-7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclohexadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.822	2.20 ng	108493	Chrysene-d12	13.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexadecane	224	C16H32	000295-65-8	97
2			Cyclotetracosane	336	C24H48	000297-03-0	95
3			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
4			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
5			1-Tetracosene	336	C24H48	010192-32-2	93

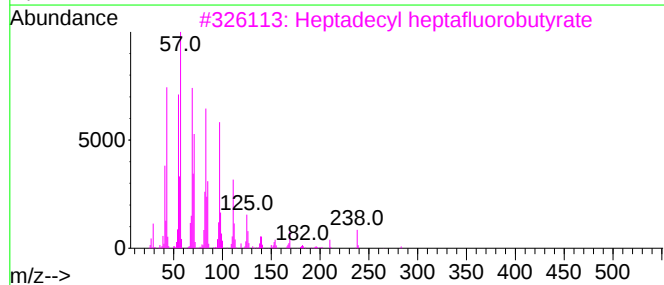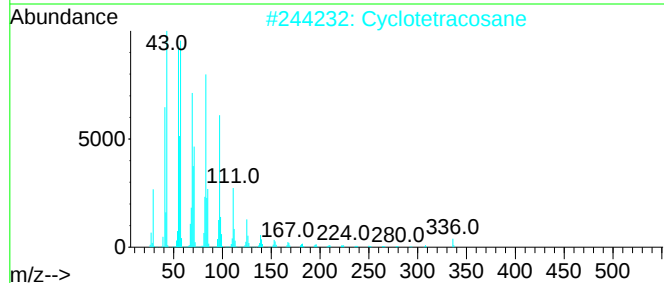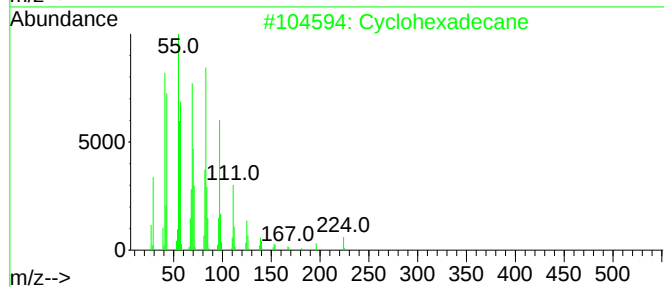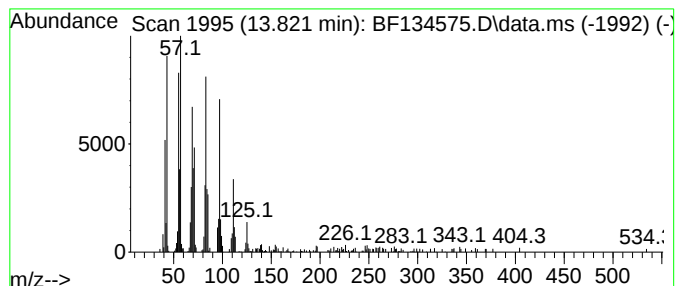

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134575.D
Acq On : 02 Aug 2023 12:26
Operator : CG\JU
Sample : 03681-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RPTP-7-CS-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclohexadecane	13.822	2.2	ng	108493	5	13.957	984422	20.0