

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
 Data File : BF134579.D
 Acq On : 02 Aug 2023 14:39
 Operator : CG\JU
 Sample : PB154346BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB154346BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.439	564	570	573	rBV	5175007	5748101	83.55%	13.302%
2	6.428	732	738	741	rBV	4547616	5909136	85.89%	13.675%
3	6.792	797	800	804	rVB	1392571	1236835	17.98%	2.862%
4	7.357	890	896	899	rBV	3538349	3888834	56.53%	8.999%
5	8.075	1012	1018	1021	rBV	1683204	1683062	24.46%	3.895%
6	9.157	1195	1202	1205	rBV	5546478	6498123	94.46%	15.038%
7	9.827	1310	1316	1319	rBV	2243304	1857640	27.00%	4.299%
8	10.621	1443	1451	1454	rBV	4095060	4113116	59.79%	9.518%
9	11.316	1559	1569	1572	rBV	2271181	1939274	28.19%	4.488%
10	12.915	1836	1841	1844	rBV	6362096	6879565	100.00%	15.920%
11	13.962	2015	2019	2022	rBV	2061076	1797088	26.12%	4.159%
12	15.427	2262	2268	2274	rVB	1356401	1661277	24.15%	3.844%




Sum of corrected areas: 43212051

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134579.D
Acq On : 02 Aug 2023 14:39
Operator : CG\JU
Sample : PB154346BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154346BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

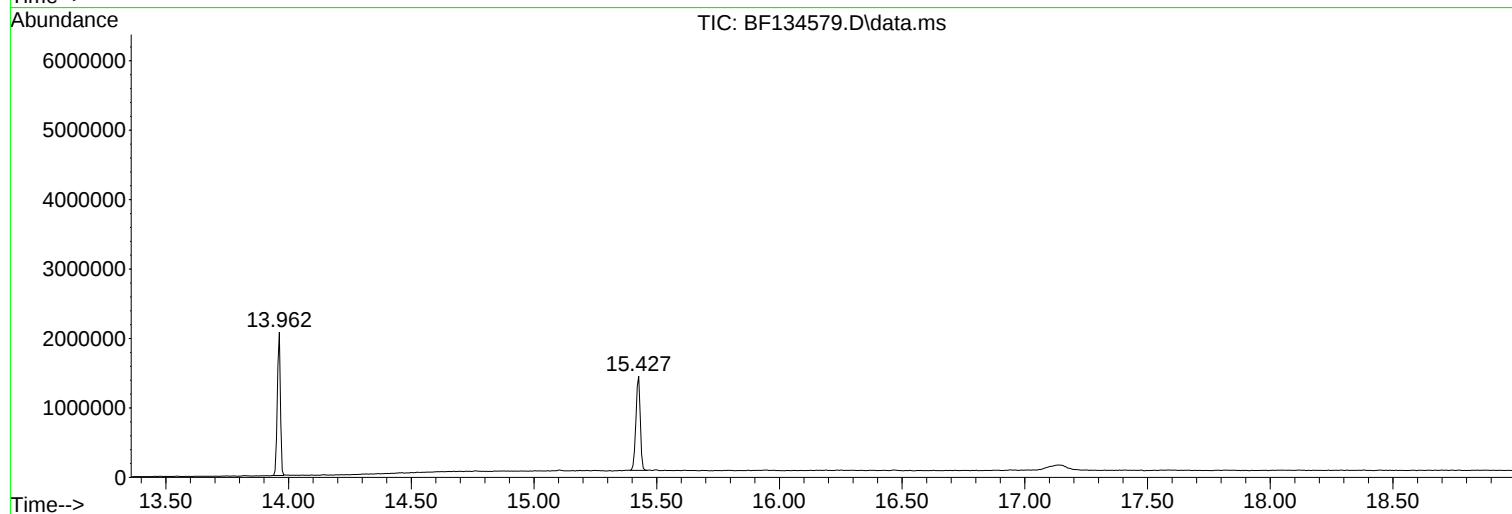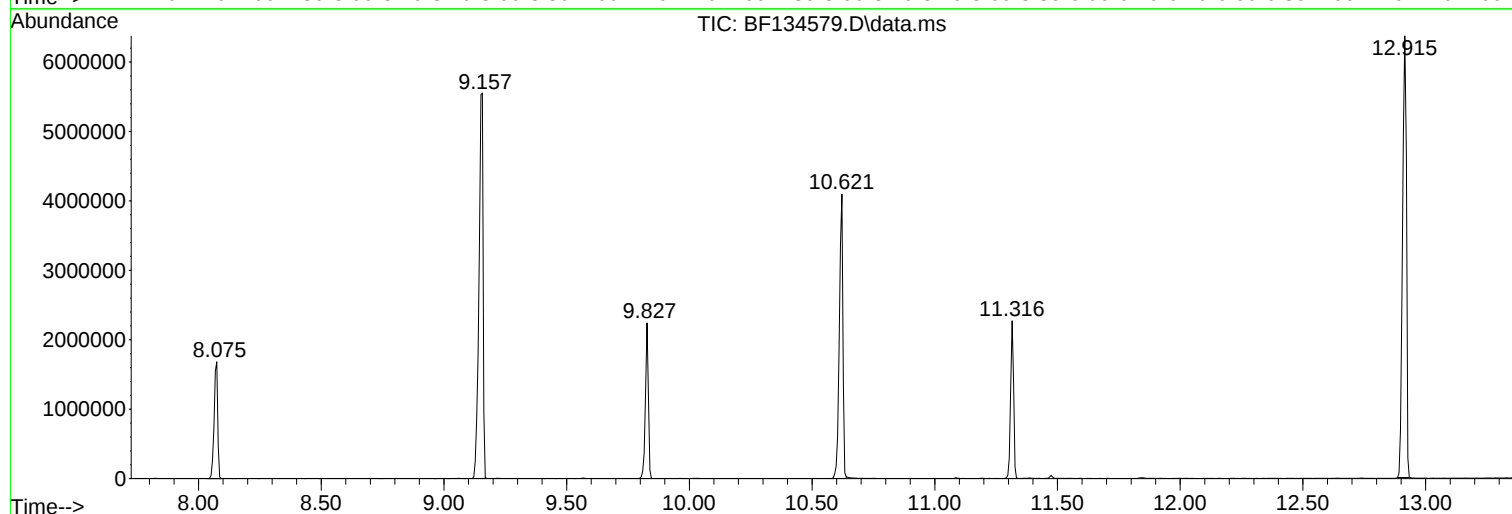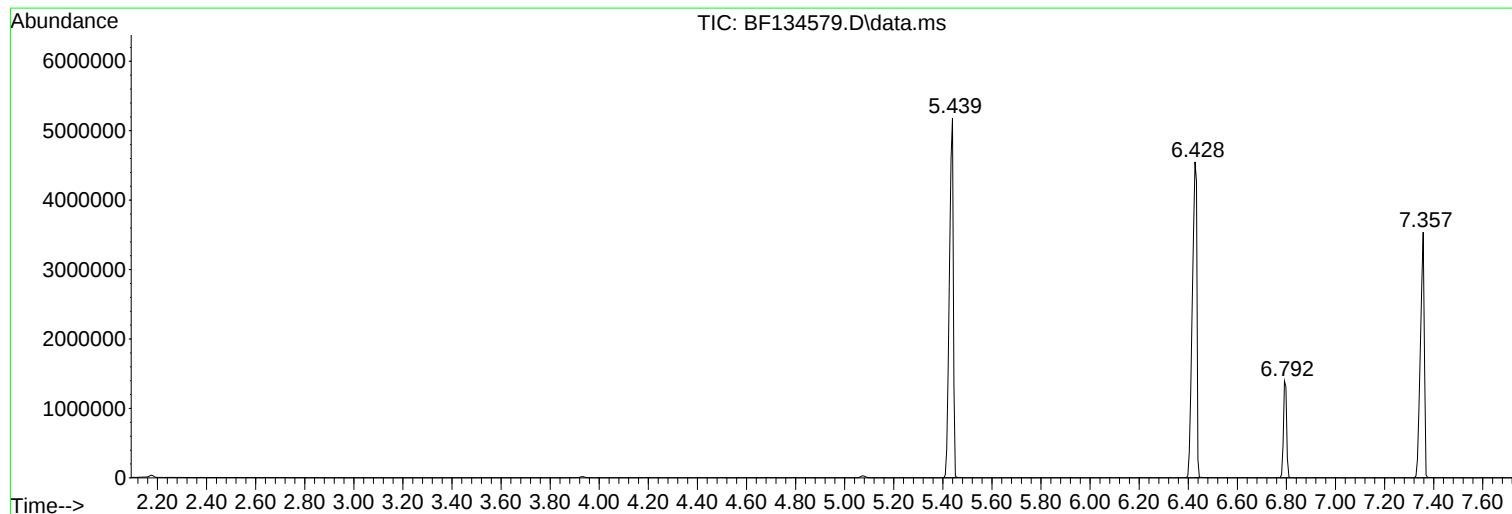

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134579.D
Acq On : 02 Aug 2023 14:39
Operator : CG\JU
Sample : PB154346BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154346BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134579.D
Acq On : 02 Aug 2023 14:39
Operator : CG\JU
Sample : PB154346BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154346BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------