

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
 Data File : BF134593.D
 Acq On : 02 Aug 2023 22:17
 Operator : CG\JU
 Sample : 03833-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 82ND-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	495	498	505	rVB	22617	26149	1.28%	0.161%
2	5.416	561	566	569	rBV	2250372	2037532	99.64%	12.574%
3	6.422	732	737	740	rBV	2203664	2044839	100.00%	12.619%
4	6.793	797	800	804	rVB	1306160	1039828	50.85%	6.417%
5	7.351	891	895	898	rBV	1569140	1207922	59.07%	7.455%
6	8.069	1014	1017	1021	rBV	1542491	1304064	63.77%	8.048%
7	9.145	1197	1200	1204	rVB	2302443	1995581	97.59%	12.315%
8	9.828	1312	1316	1319	rBV	1357380	1178682	57.64%	7.274%
9	10.610	1445	1449	1453	rBV	1262155	1014712	49.62%	6.262%
10	11.310	1565	1568	1572	rBV	1182486	1038047	50.76%	6.406%
11	11.845	1656	1659	1664	rBV	36760	40111	1.96%	0.248%
12	12.904	1835	1839	1843	rBV	1976705	1655326	80.95%	10.216%
13	13.822	1991	1995	2002	rBV	79798	94103	4.60%	0.581%
14	13.957	2014	2018	2022	rBV	1045942	849164	41.53%	5.240%
15	14.451	2098	2102	2107	rBV4	14560	28785	1.41%	0.178%
16	15.421	2262	2267	2274	rVB	522270	649032	31.74%	4.005%




Sum of corrected areas: 16203877

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134593.D
Acq On : 02 Aug 2023 22:17
Operator : CG\JU
Sample : 03833-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
82ND-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

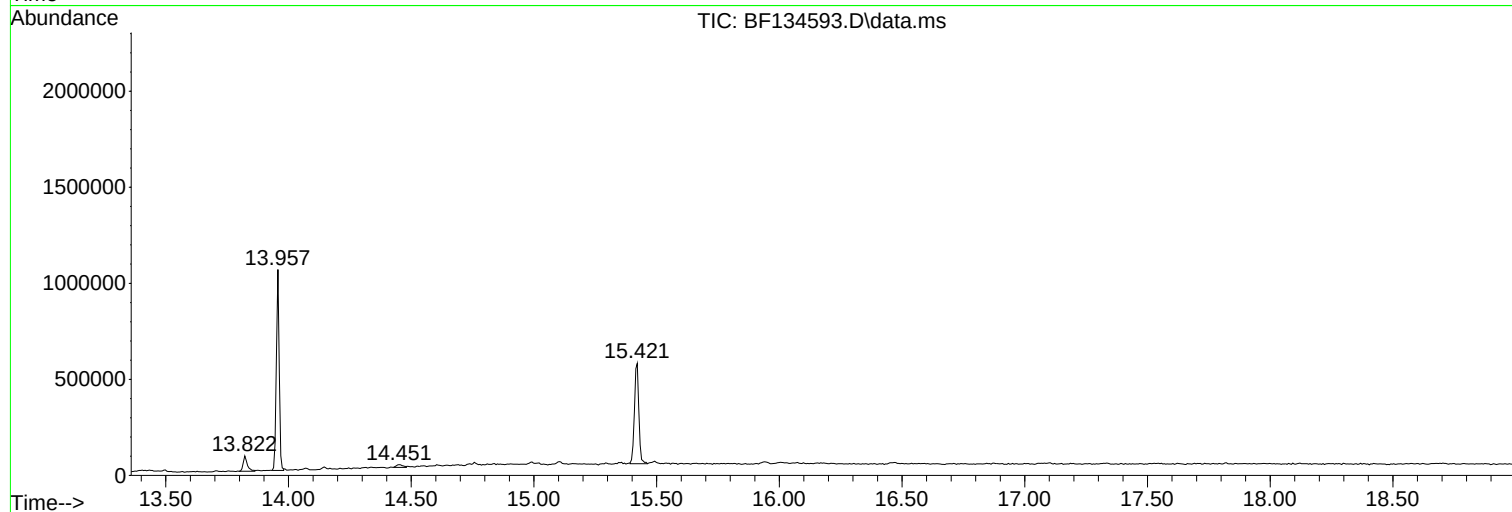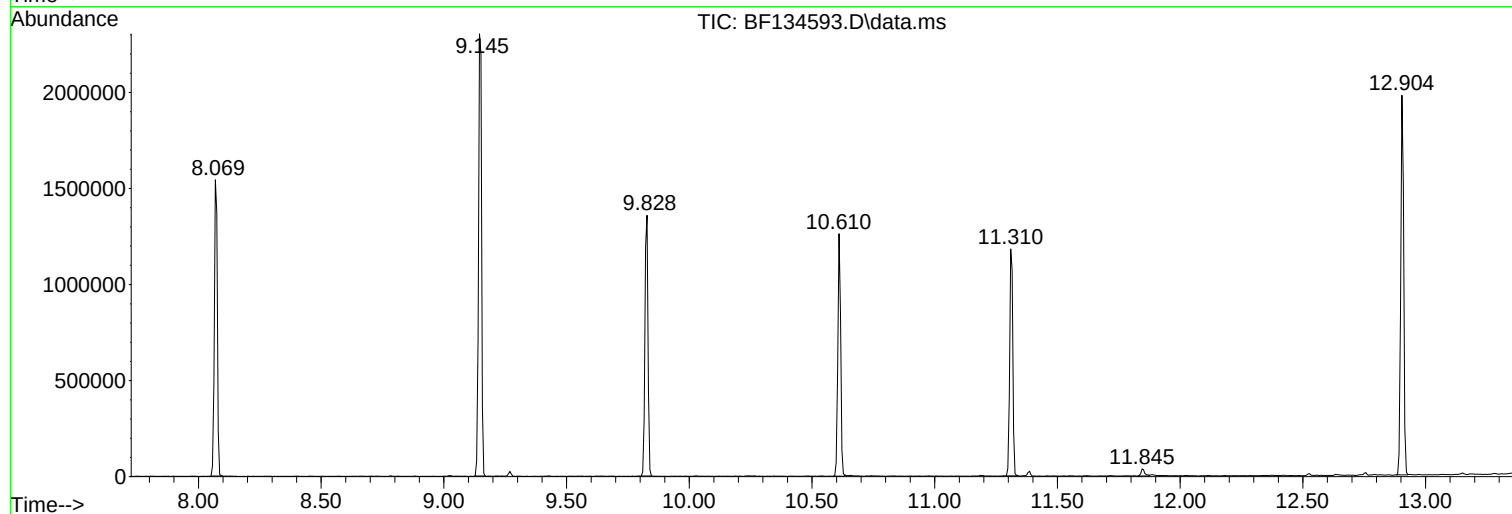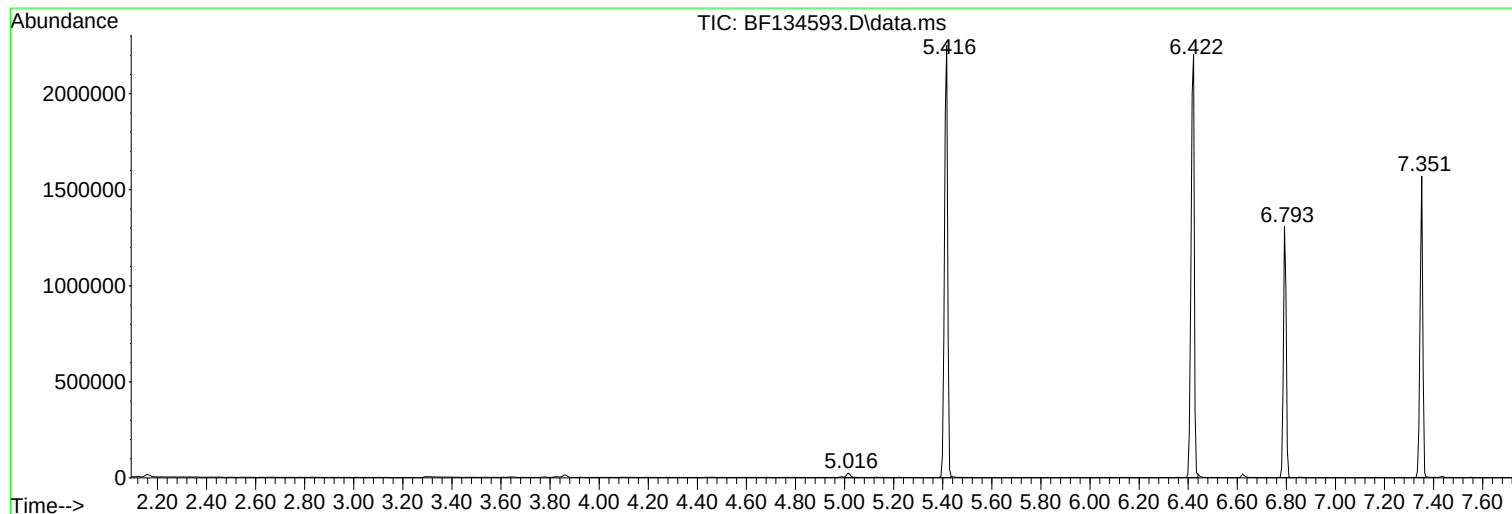

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134593.D
Acq On : 02 Aug 2023 22:17
Operator : CG\JU
Sample : 03833-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
82ND-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Heptadecyl heptafluorobutyrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.822	2.22 ng	94103	Chrysene-d12	13.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	95
2			1-Heneicosanol	312	C21H44O	015594-90-8	93
3			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	91
4			Octadecyl trifluoroacetate	366	C20H37F3O2	079392-43-1	91
5			Docosyl pentafluoropropionate	472	C25H45F5O2	1000351-80-9	91

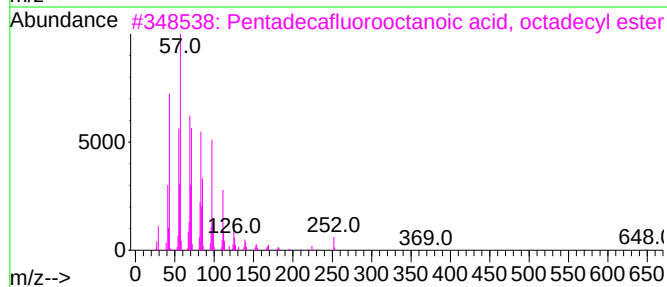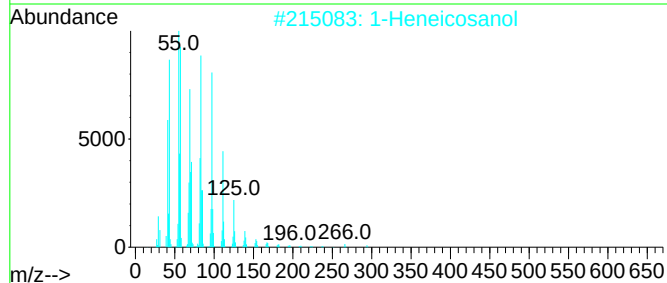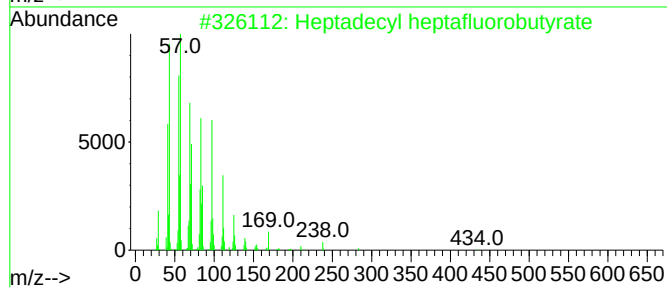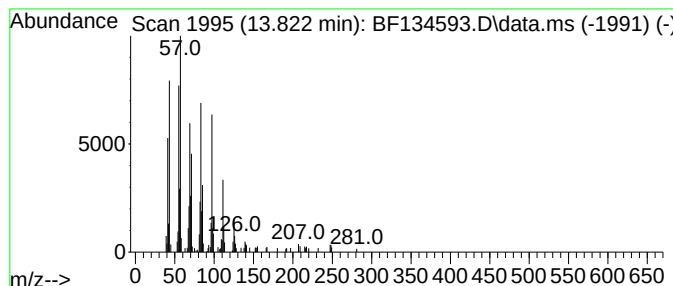

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134593.D
Acq On : 02 Aug 2023 22:17
Operator : CG\JU
Sample : 03833-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
82ND-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Heptadecyl hept...	13.822	2.2	ng	94103	5	13.957	849164	20.0