


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134567.D
Acq On : 02 Aug 2023 08:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 02 02:20:34 2023

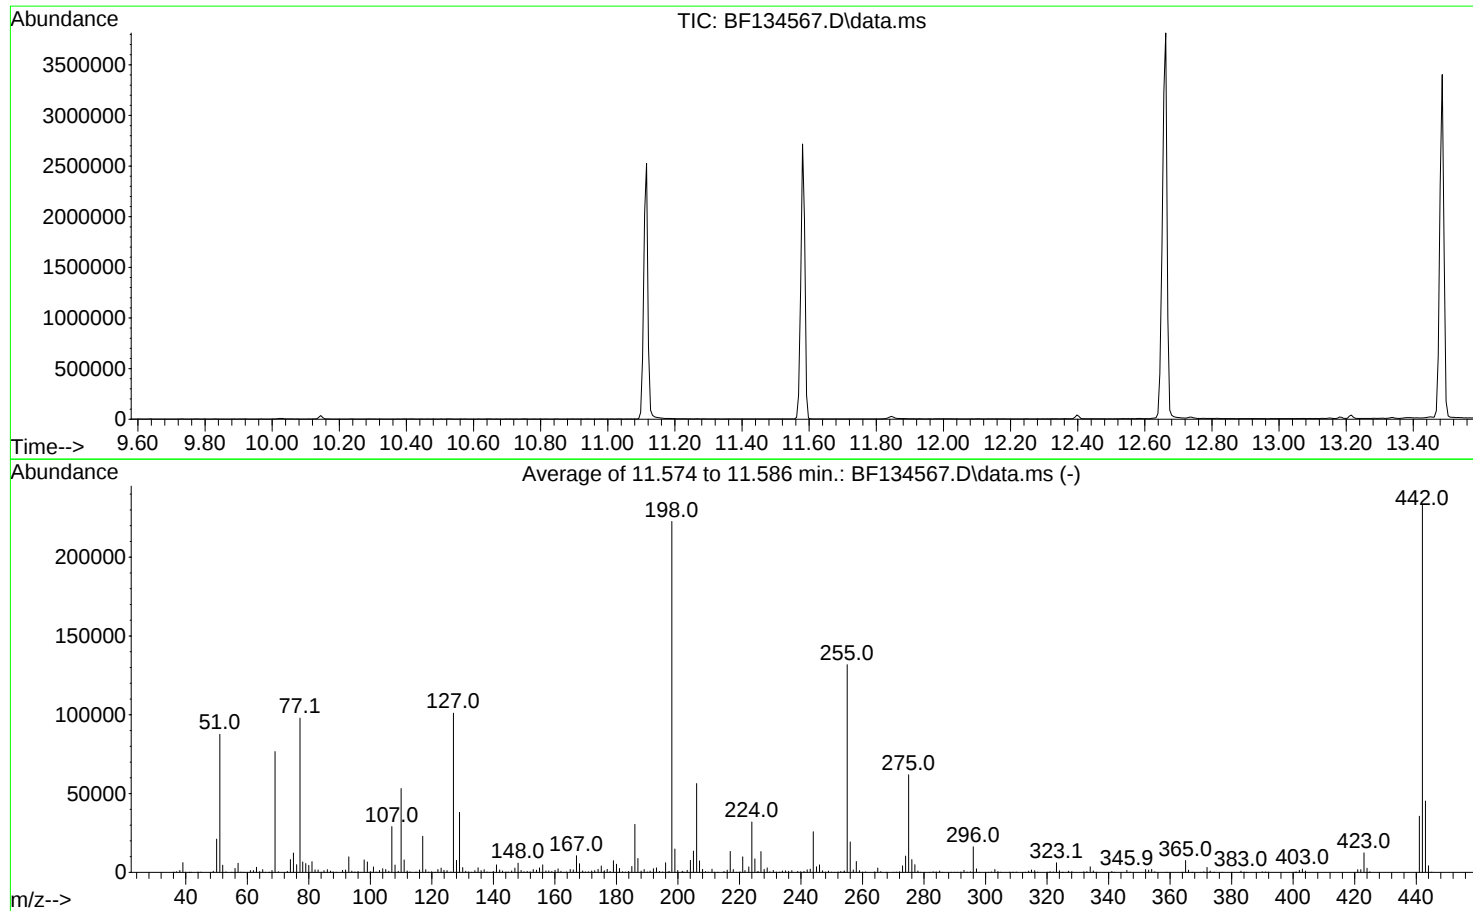




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	87592	PASS
68	69	0.00	2	1.6	1261	PASS
69	198	0.00	100	34.4	76621	PASS
70	69	0.00	2	0.6	424	PASS
127	198	10	80	45.4	101021	PASS
197	198	0.00	2	0.3	581	PASS
198	198	100	100	100.0	222656	PASS
199	198	5	9	6.7	14857	PASS
275	198	10	60	27.8	61965	PASS
365	198	1	100	3.4	7511	PASS
441	198	0.01	100	16.0	35684	PASS
442	442	50	100	100.0	233427	PASS
443	442	15	24	19.4	45271	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134567.D
Acq On : 02 Aug 2023 08:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 18:34:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

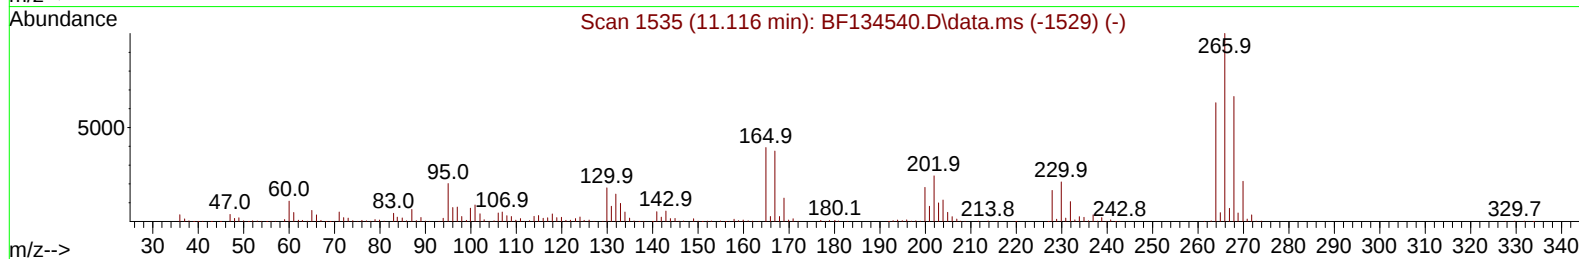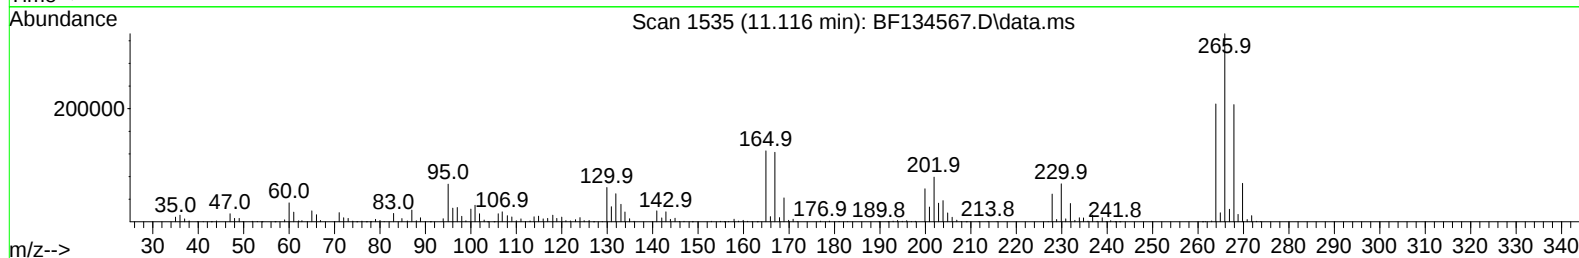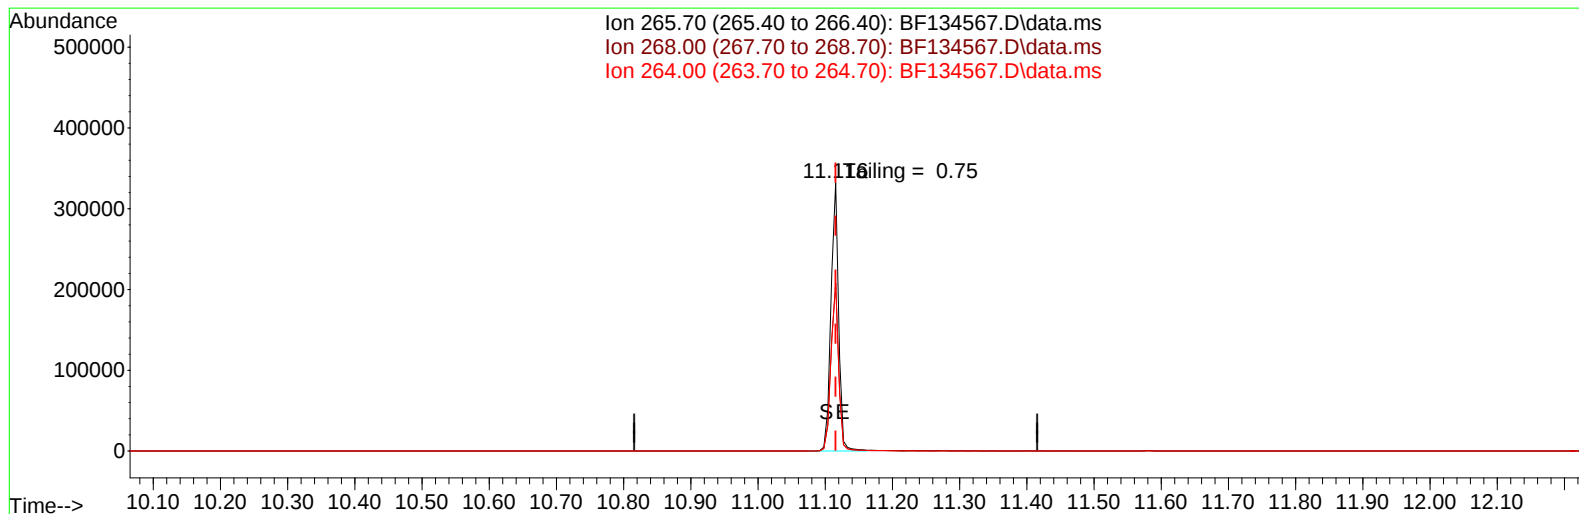

TIC: BF134567.D\data.ms

(70) Pentachlorophenol (C)

11.116min (+ 0.000) 611186.26 ng




response 266843

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.35
264.00	59.70	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134567.D
Acq On : 02 Aug 2023 08:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 18:34:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

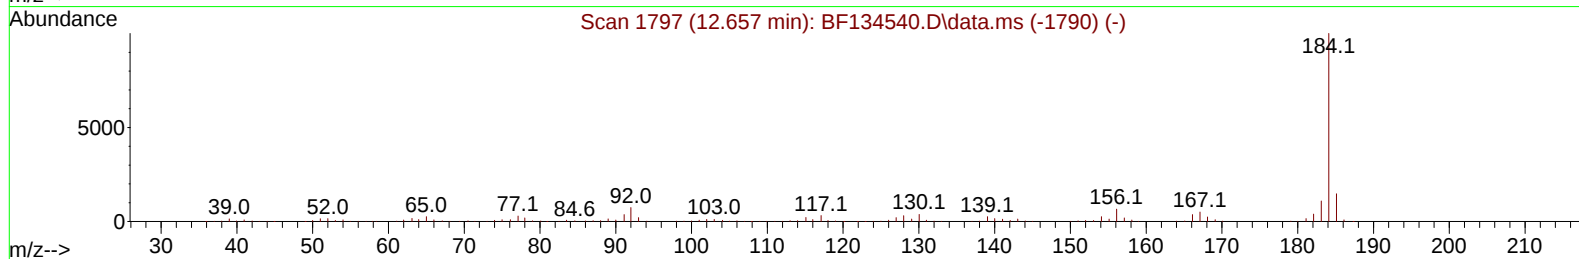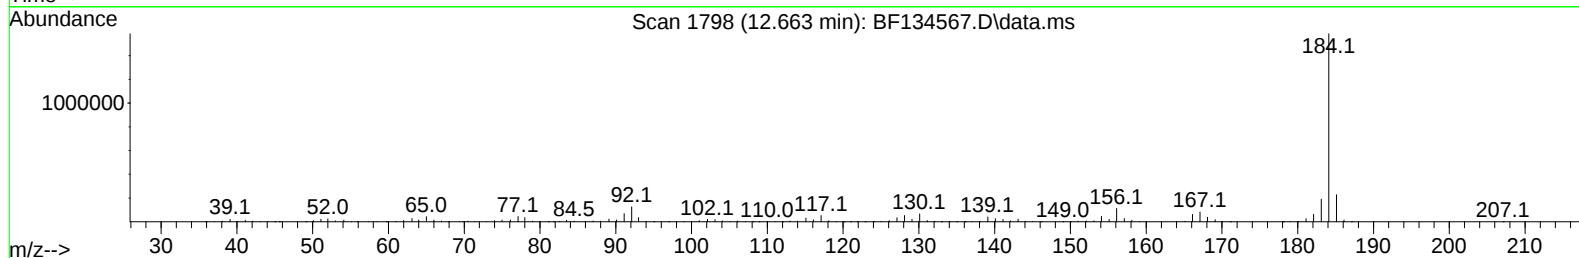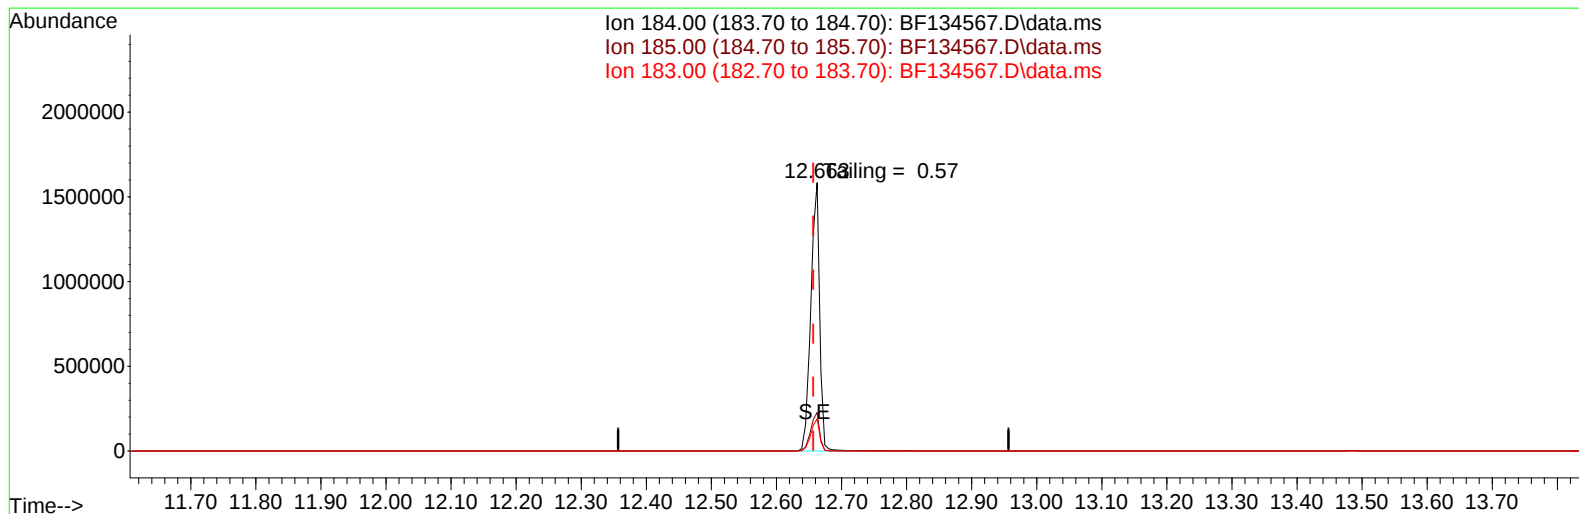

TIC: BF134567.D\data.ms

(77) Benzidine

12.663min (+ 0.006) 623264.74 ng

response 1501803

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.36
183.00	10.80	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2023	BNA_F	<u>BF134567.D</u>
Compound Name	Response	Retention Time
DDT	567759	13.486
DDD	7130	13.215
DDE	115	12.815
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7245	575004	1.26

Instrument :
BNA_F
ClientSampleId :
DFTPP