
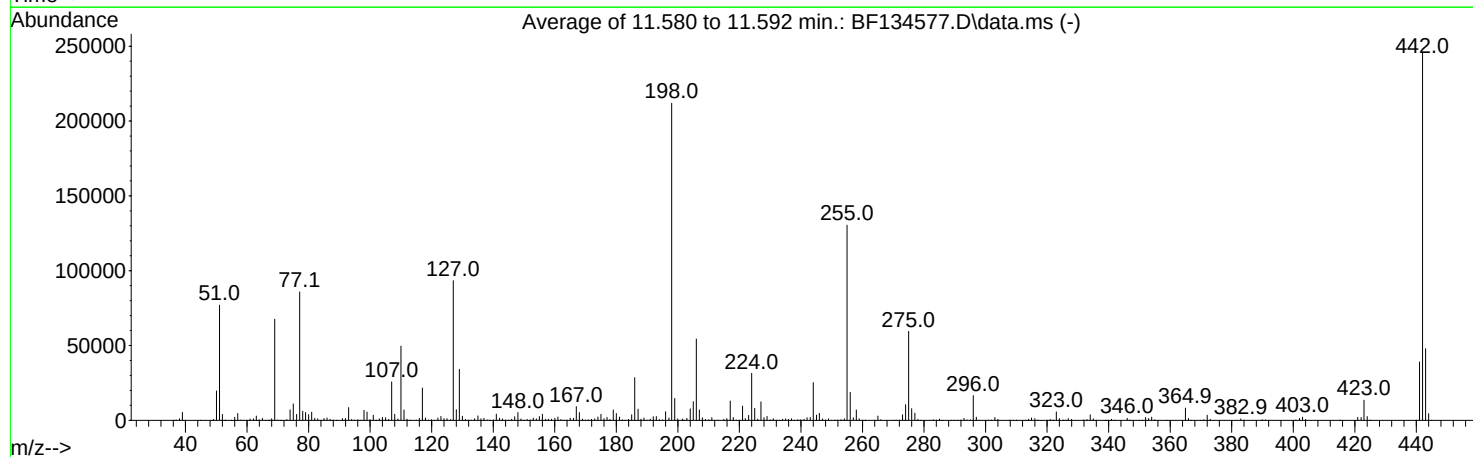


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134577.D
Acq On : 02 Aug 2023 13:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 02 02:20:34 2023

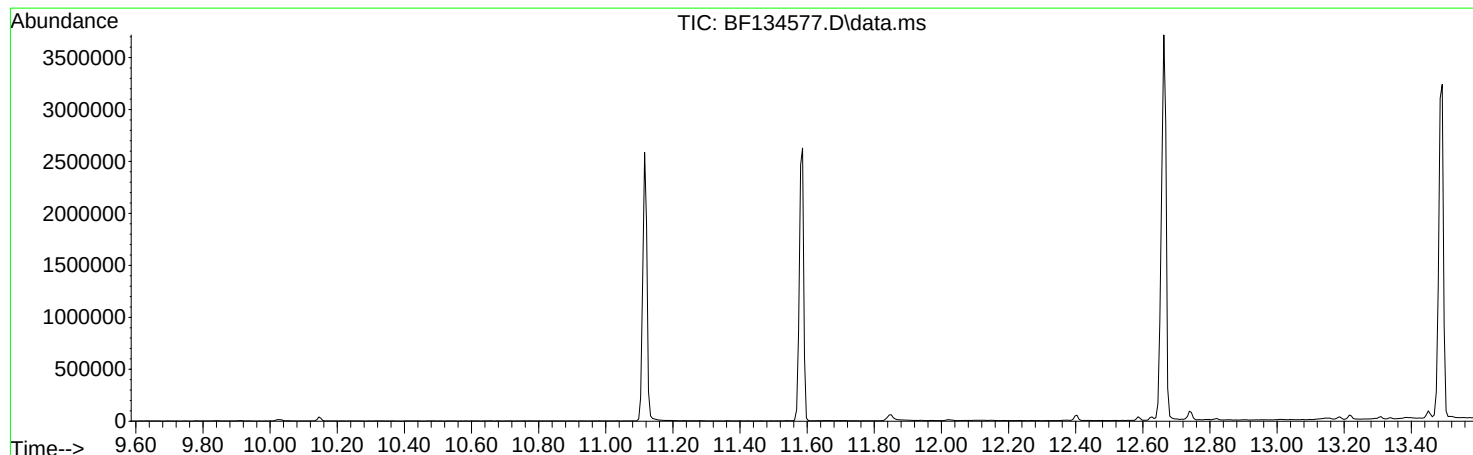




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	77034	PASS
68	69	0.00	2	1.7	1127	PASS
69	198	0.00	100	31.9	67563	PASS
70	69	0.00	2	0.3	201	PASS
127	198	10	80	44.0	93309	PASS
197	198	0.00	2	0.8	1658	PASS
198	198	100	100	100.0	211888	PASS
199	198	5	9	6.9	14627	PASS
275	198	10	60	28.0	59405	PASS
365	198	1	100	3.9	8269	PASS
441	198	0.01	100	18.4	39008	PASS
442	442	50	100	100.0	245803	PASS
443	442	15	24	19.5	47896	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
Data File : BF134577.D
Acq On : 02 Aug 2023 13:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 15:38:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

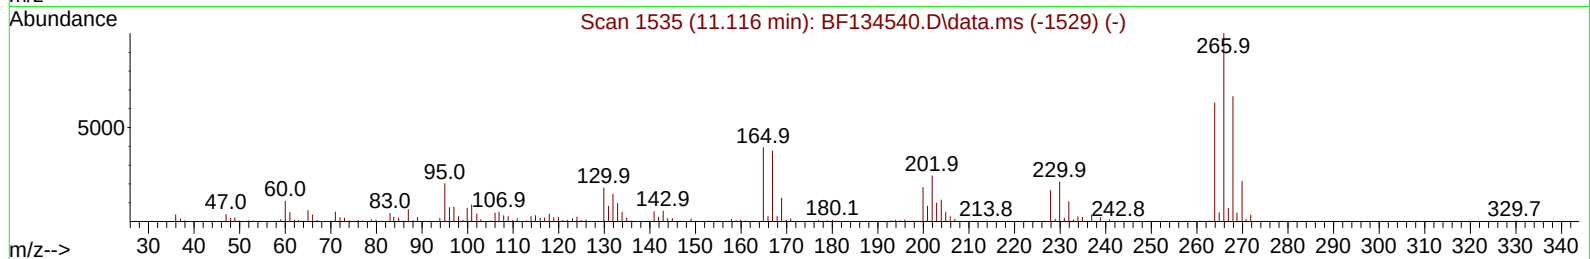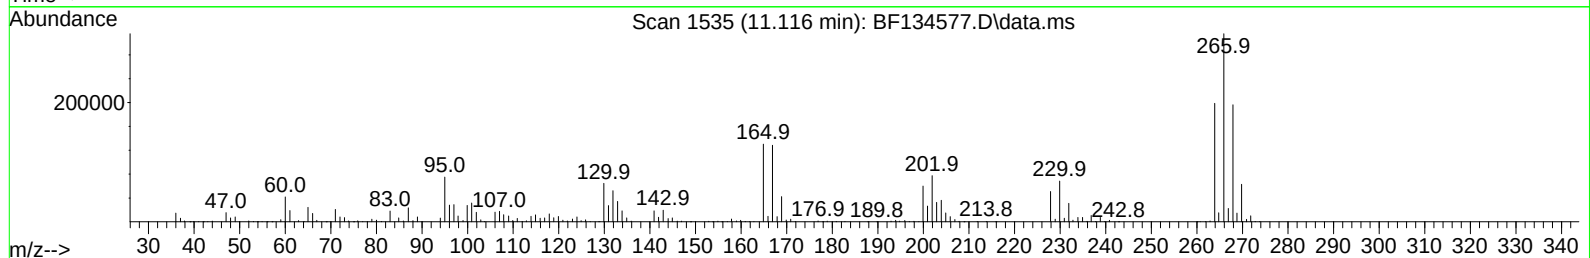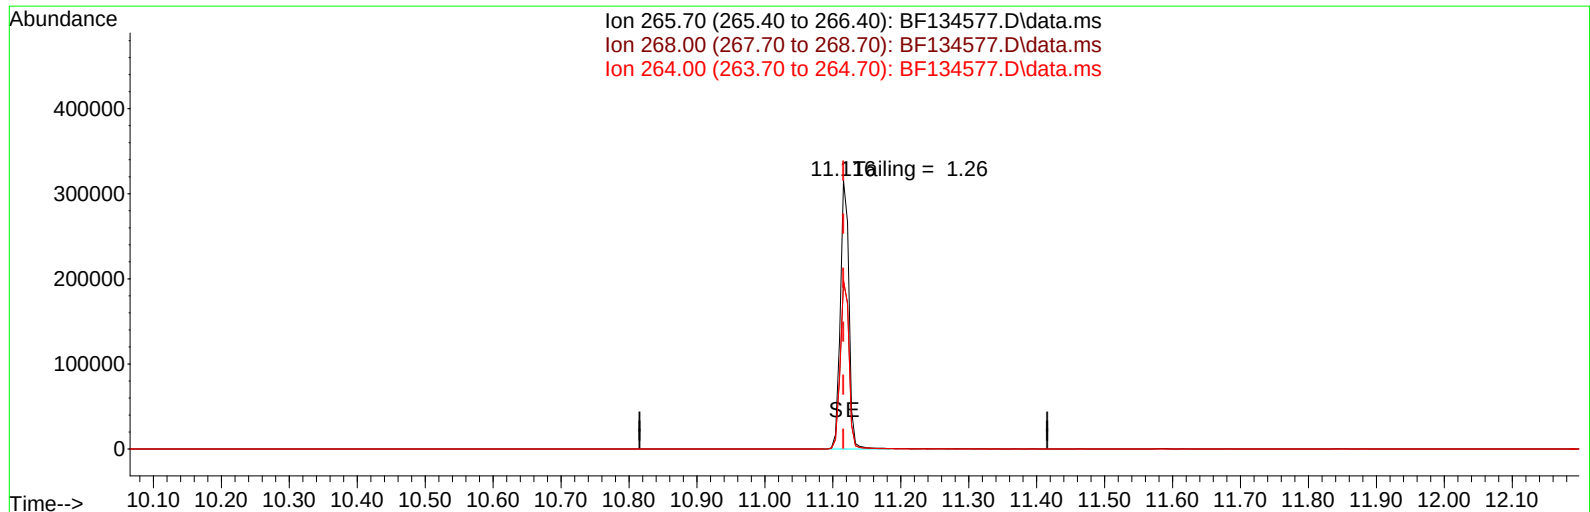

TIC: BF134577.D\data.ms

(70) Pentachlorophenol (C)

11.116min (+ 0.000) 536612.68 ng




response 280373

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.26
264.00	59.70	62.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080223\
 Data File : BF134577.D
 Acq On : 02 Aug 2023 13:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 02 15:38:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 02 02:20:34 2023
 Response via : Initial Calibration

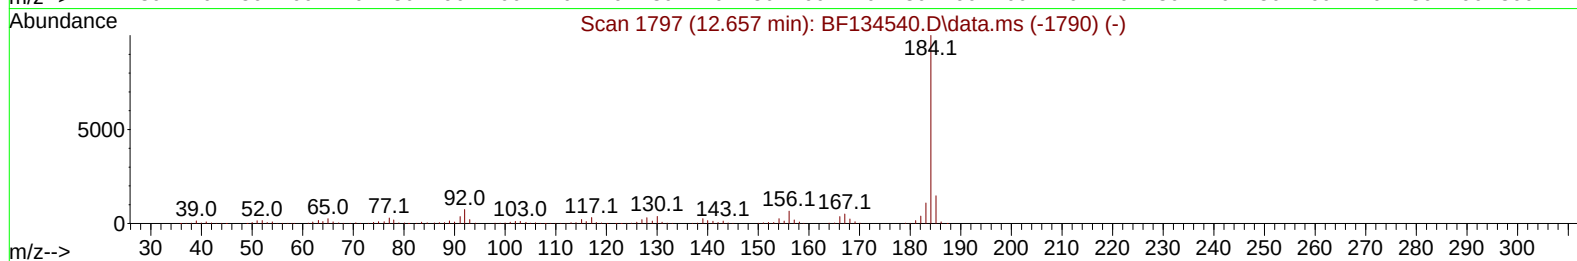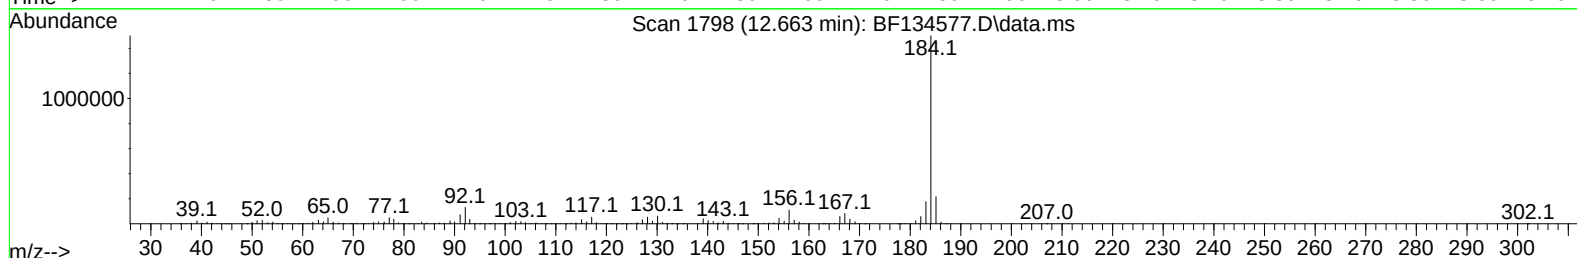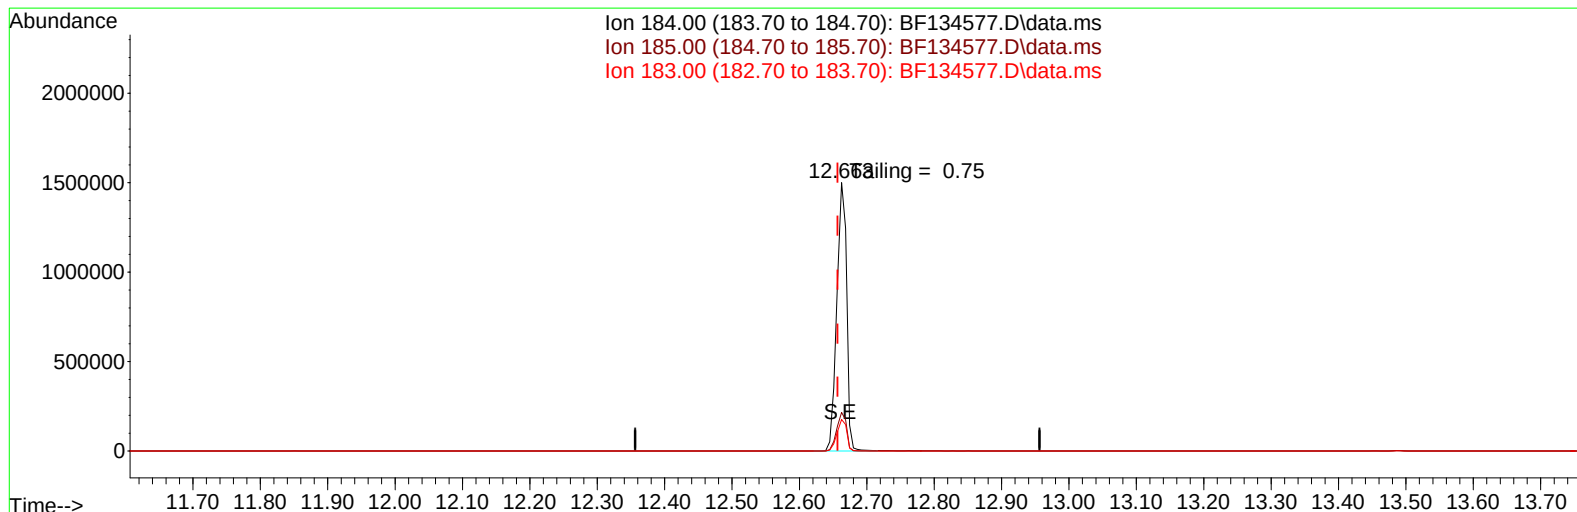

TIC: BF134577.D\data.ms

(77) Benzidine

12.663min (+ 0.006) 240370.22 ng

response 1523635

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.41
183.00	10.80	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2023	BNA_F	<u>BF134577.D</u>
Compound Name	Response	Retention Time
DDT	612667	13.492
DDD	9262	13.215
DDE	151	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9413	622080	1.51

Instrument :
BNA_F
ClientSampleId :
DFTPP