


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080319\
 Data File : BF115969.D
 Acq On : 3 Aug 2019 9:13
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 31 15:31:51 2019

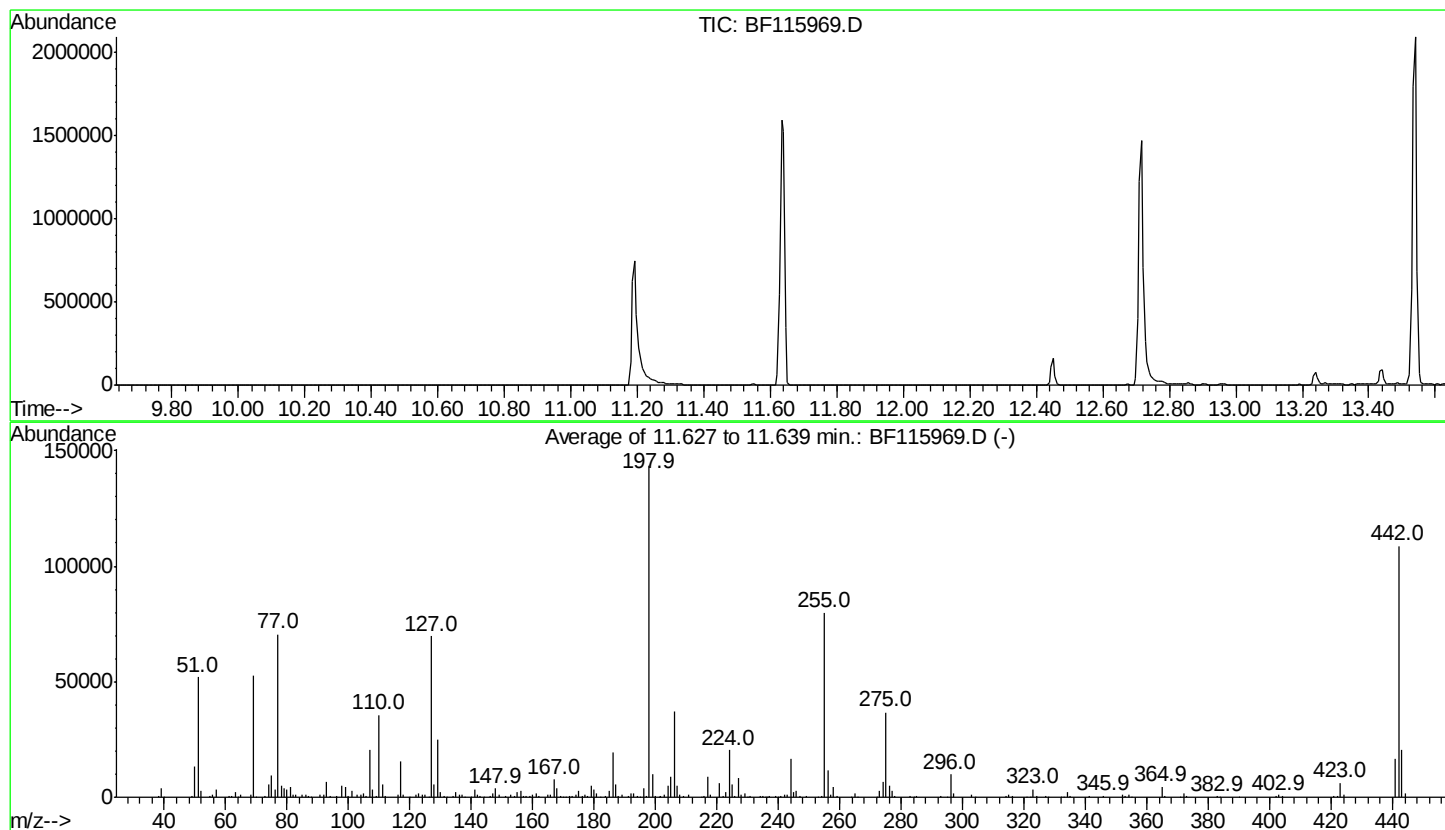

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	51853	PASS
68	69	0.00	2	1.7	911	PASS
69	198	0.00	100	36.8	52880	PASS
70	69	0.00	2	0.3	167	PASS
127	198	10	80	48.5	69594	PASS
197	198	0.00	2	0.6	812	PASS
198	198	100	100	100.0	143522	PASS
199	198	5	9	6.9	9940	PASS
275	198	10	60	25.7	36836	PASS
365	198	1	100	3.2	4528	PASS
441	198	0.01	100	11.7	16789	PASS
442	198	50	100	75.7	108690	PASS
443	442	15	24	18.8	20473	PASS