
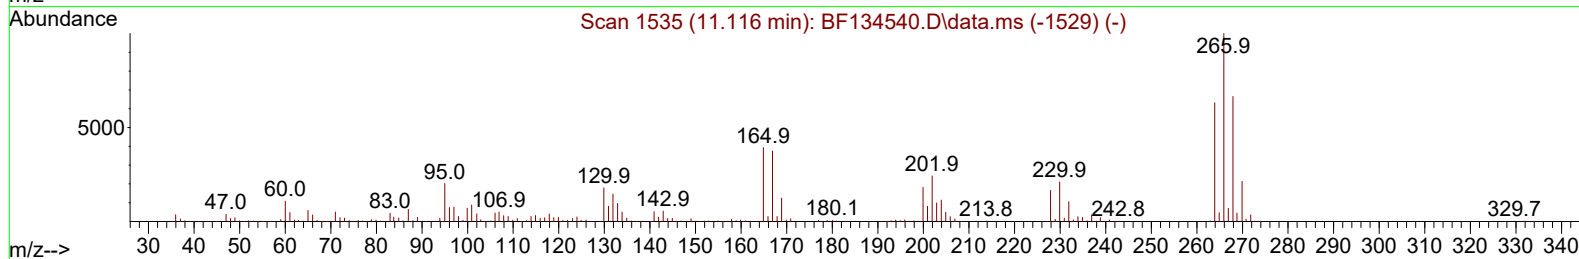
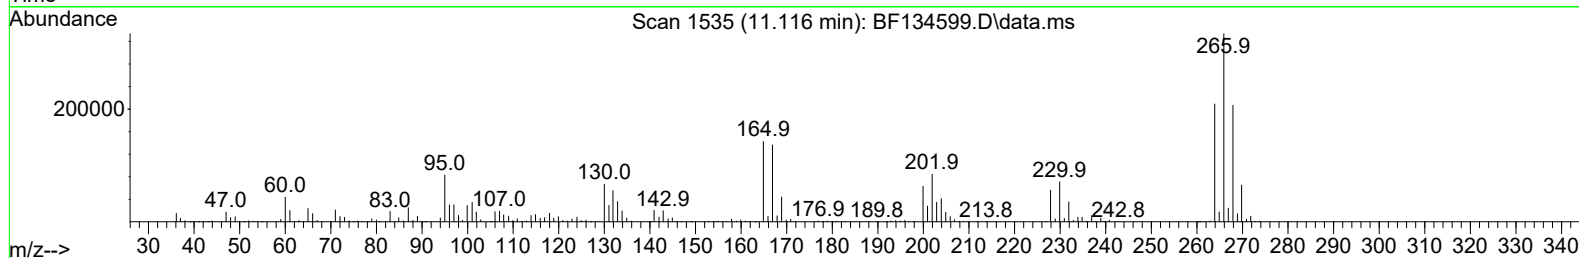


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
Data File : BF134599.D
Acq On : 03 Aug 2023 08:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 14:47:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

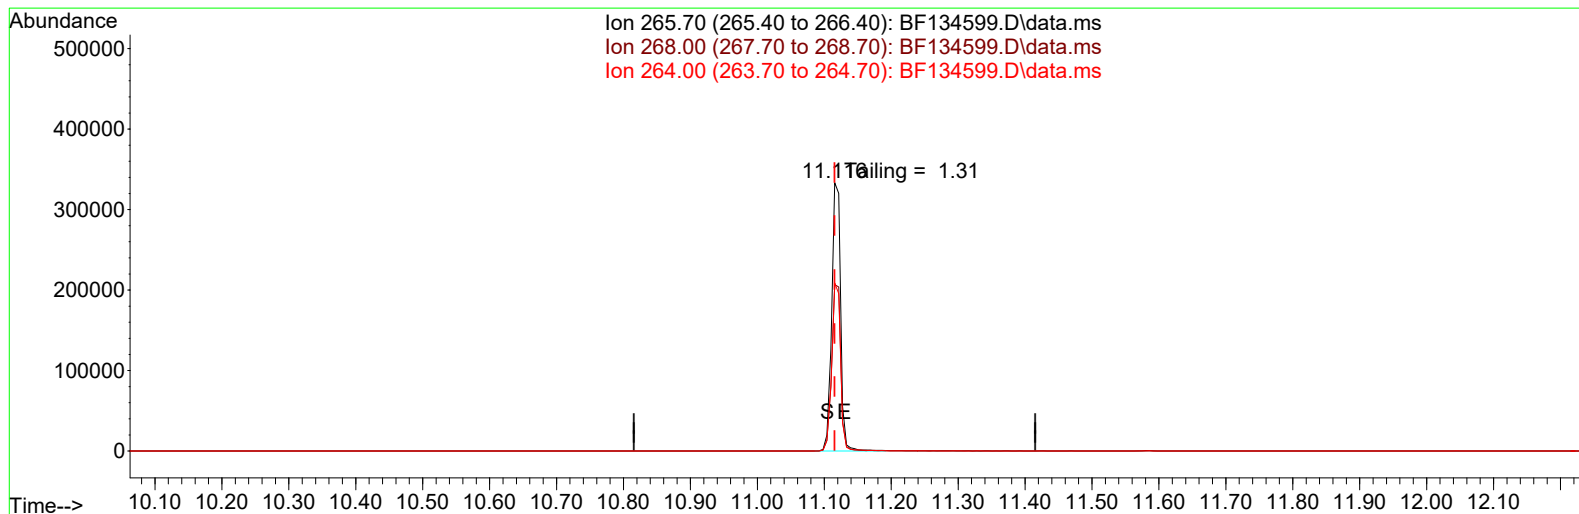

TIC: BF134599.D\data.ms

(70) Pentachlorophenol (C)




11.116min (+ 0.000) 191005.28 ng

response 311697

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.00
264.00	59.70	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
Data File : BF134599.D
Acq On : 03 Aug 2023 08:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 14:47:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

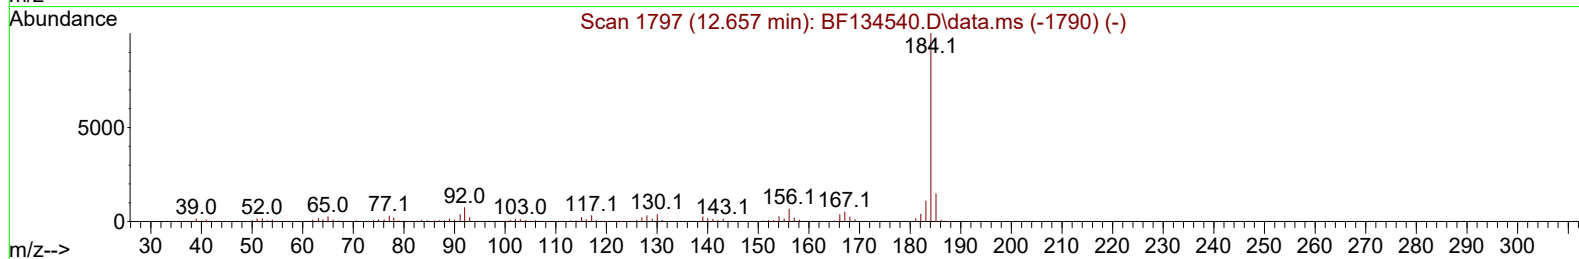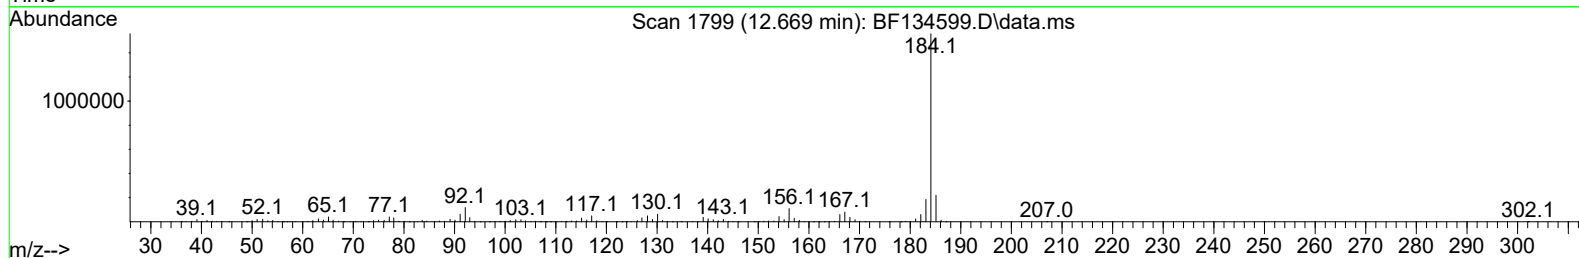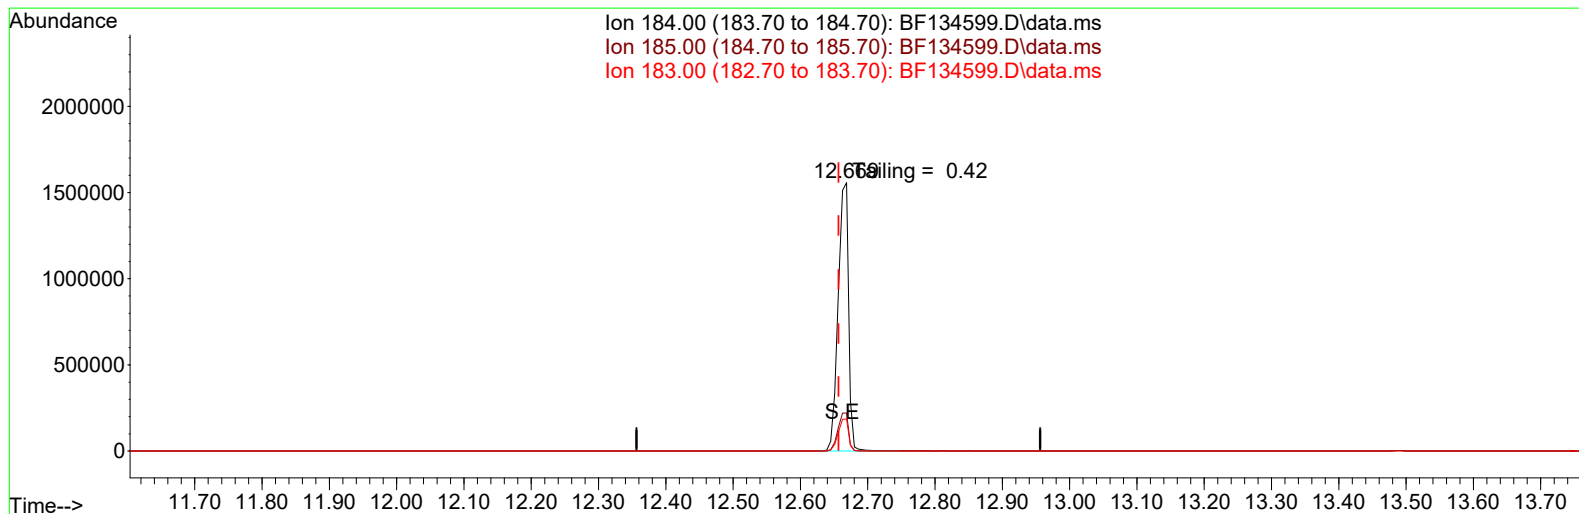

TIC: BF134599.D\data.ms

(77) Benzidine**12.669min (+ 0.012) 588780.03 ng****response 1687114**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.16
183.00	10.80	11.92
0.00	0.00	0.00