

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
Data File : BF134601.D
Acq On : 03 Aug 2023 09:14
Operator : CG\JU
Sample : PB154404BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154404BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.181	8	16	21	rVB	78142	111653	1.64%	0.263%
2	5.439	564	570	573	rBV	5080332	5536315	81.51%	13.034%
3	6.428	732	738	741	rBV	4390098	5702137	83.95%	13.425%
4	6.792	797	800	804	rVB	1396449	1233712	18.16%	2.905%
5	7.357	890	896	899	rBV	3355977	3687785	54.29%	8.682%
6	8.075	1012	1018	1021	rBV	1684882	1678021	24.70%	3.951%
7	9.151	1195	1201	1204	rBV	5596668	6226592	91.67%	14.659%
8	9.827	1310	1316	1319	rBV	2230390	1874235	27.59%	4.413%
9	10.616	1443	1450	1454	rBV	3737382	4079596	60.06%	9.605%
10	11.316	1563	1569	1572	rBV	2466026	1996776	29.40%	4.701%
11	12.915	1833	1841	1844	rBV	6219978	6792361	100.00%	15.991%
12	13.962	2014	2019	2022	rBV	2082686	1818865	26.78%	4.282%
13	15.427	2262	2268	2273	rBV	1383615	1737516	25.58%	4.091%




Sum of corrected areas: 42475564

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
Data File : BF134601.D
Acq On : 03 Aug 2023 09:14
Operator : CG\JU
Sample : PB154404BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154404BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

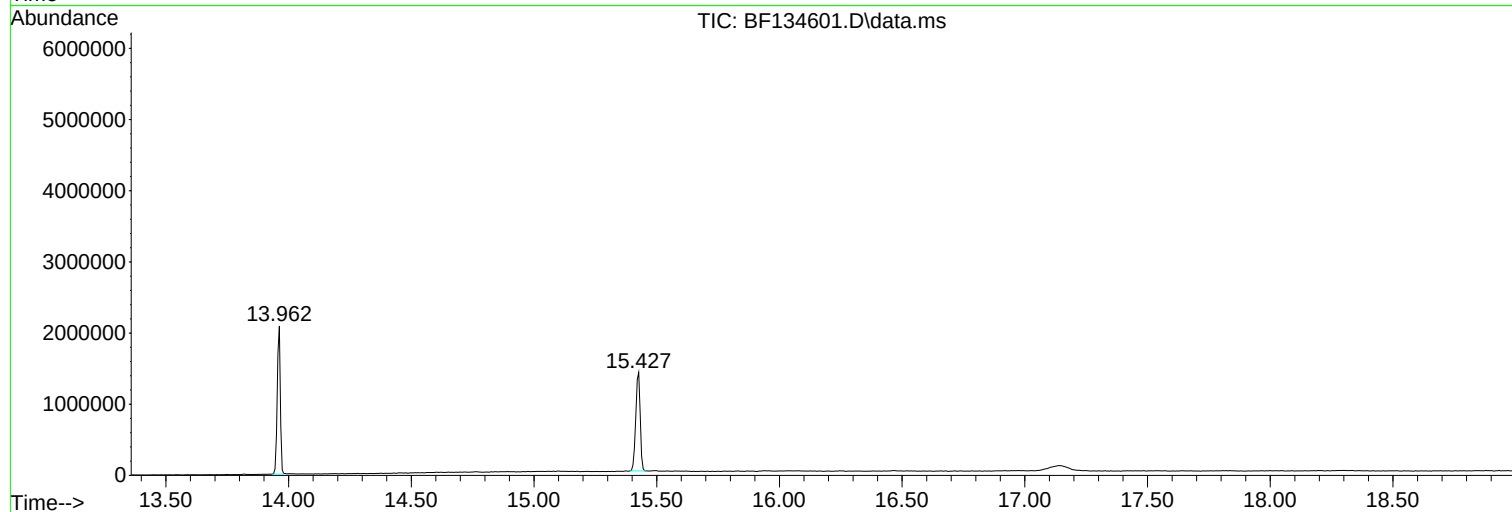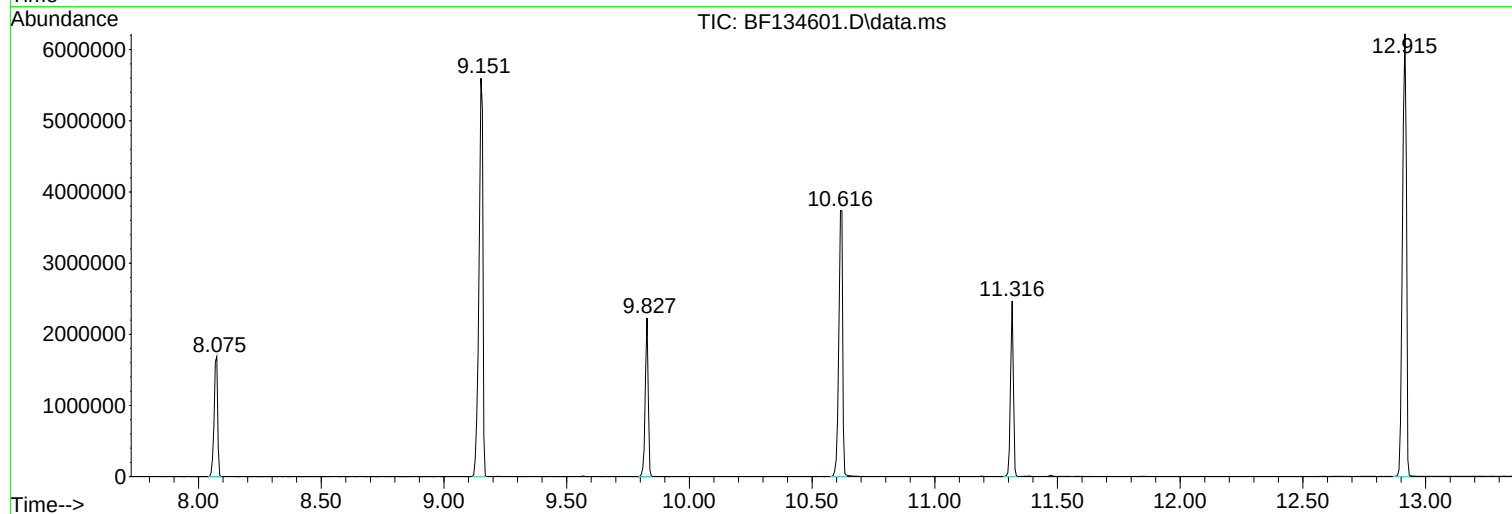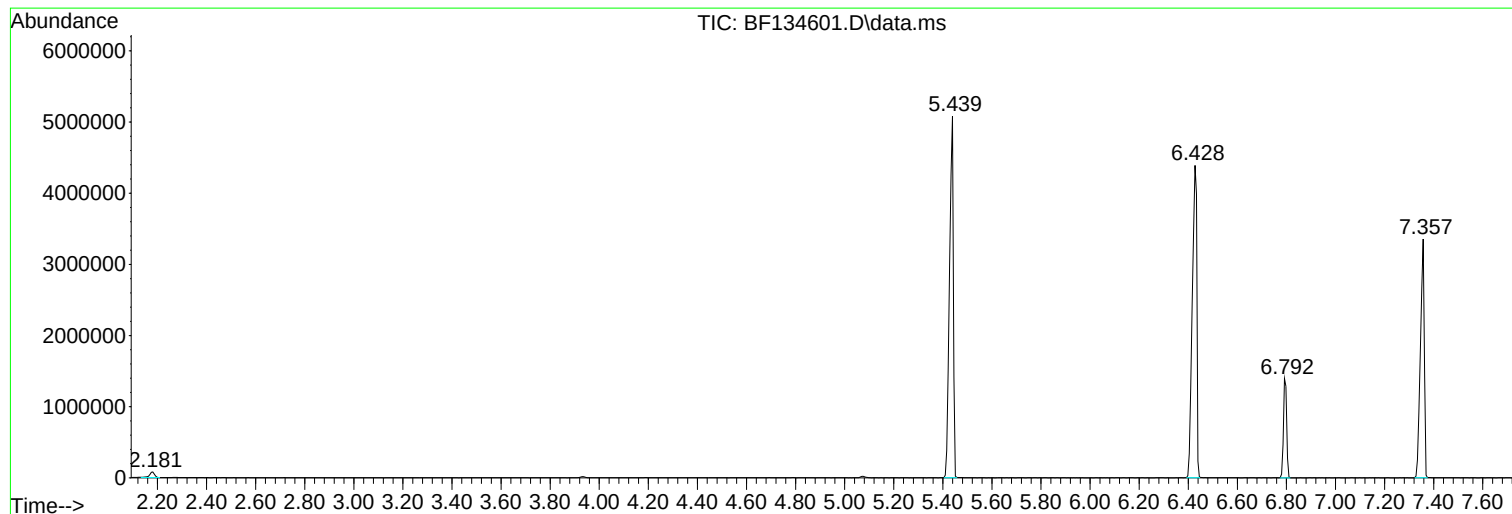

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
Data File : BF134601.D
Acq On : 03 Aug 2023 09:14
Operator : CG\JU
Sample : PB154404BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154404BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
Data File : BF134601.D
Acq On : 03 Aug 2023 09:14
Operator : CG\JU
Sample : PB154404BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154404BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------