

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
 Data File : BF134612.D
 Acq On : 03 Aug 2023 15:42
 Operator : CG\JU
 Sample : 03756-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RPTP-9-CS-9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134613.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	6	11	24	rVB2	32887	53717	2.89%	0.342%
2	5.016	495	498	504	rVB	19720	24728	1.33%	0.157%
3	5.422	562	567	570	rBV	1937472	1856284	100.00%	11.802%
4	6.422	733	737	740	rBV	1973046	1807393	97.37%	11.491%
5	6.622	768	771	777	rBV	60594	57552	3.10%	0.366%
6	6.798	797	801	804	rBV	1279351	968473	52.17%	6.157%
7	7.357	891	896	899	rBV	1204420	1032146	55.60%	6.562%
8	8.075	1014	1018	1022	rBV	1518612	1164958	62.76%	7.406%
9	9.151	1197	1201	1204	rBV	2327348	1831391	98.66%	11.643%
10	9.269	1218	1221	1225	rVB	34054	31471	1.70%	0.200%
11	9.828	1313	1316	1320	rBV	1281819	1129655	60.86%	7.182%
12	10.616	1447	1450	1454	rBV	1247716	1058503	57.02%	6.730%
13	11.322	1566	1570	1573	rBV	1329802	1205431	64.94%	7.664%
14	11.386	1576	1581	1585	rVV3	31364	35861	1.93%	0.228%
15	11.857	1657	1661	1664	rBV2	95061	105493	5.68%	0.671%
16	12.533	1773	1776	1779	rBV	44575	43081	2.32%	0.274%
17	12.763	1813	1815	1819	rVB	43527	39821	2.15%	0.253%
18	12.910	1837	1840	1844	rBV	1971010	1744835	94.00%	11.093%
19	13.821	1992	1995	2001	rBV3	196326	223052	12.02%	1.418%
20	13.968	2016	2020	2023	rVB	793758	700179	37.72%	4.451%
21	15.439	2266	2270	2279	rVB	433048	615129	33.14%	3.911%




Sum of corrected areas: 15729153

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
Data File : BF134612.D
Acq On : 03 Aug 2023 15:42
Operator : CG\JU
Sample : 03756-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RPTP-9-CS-9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

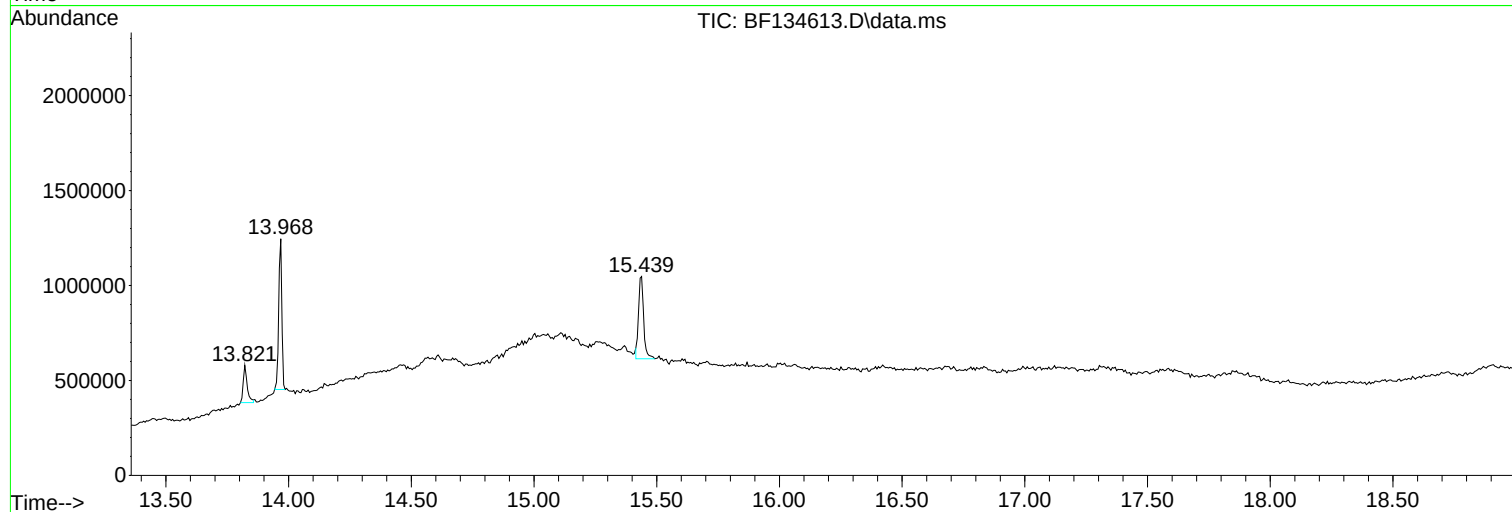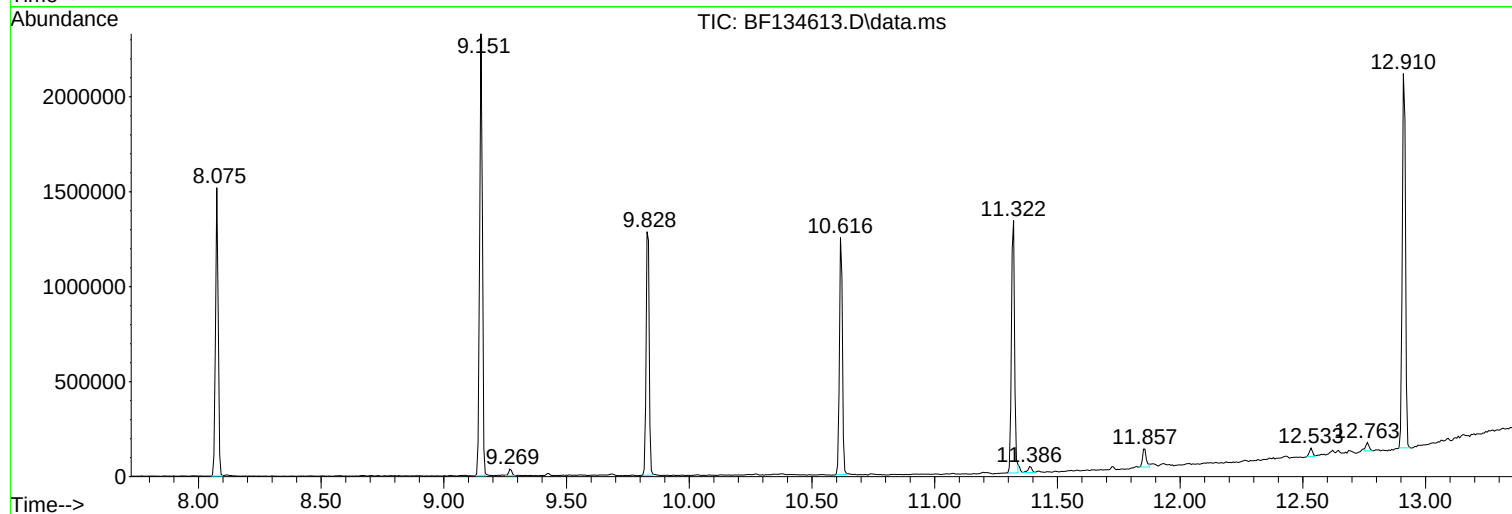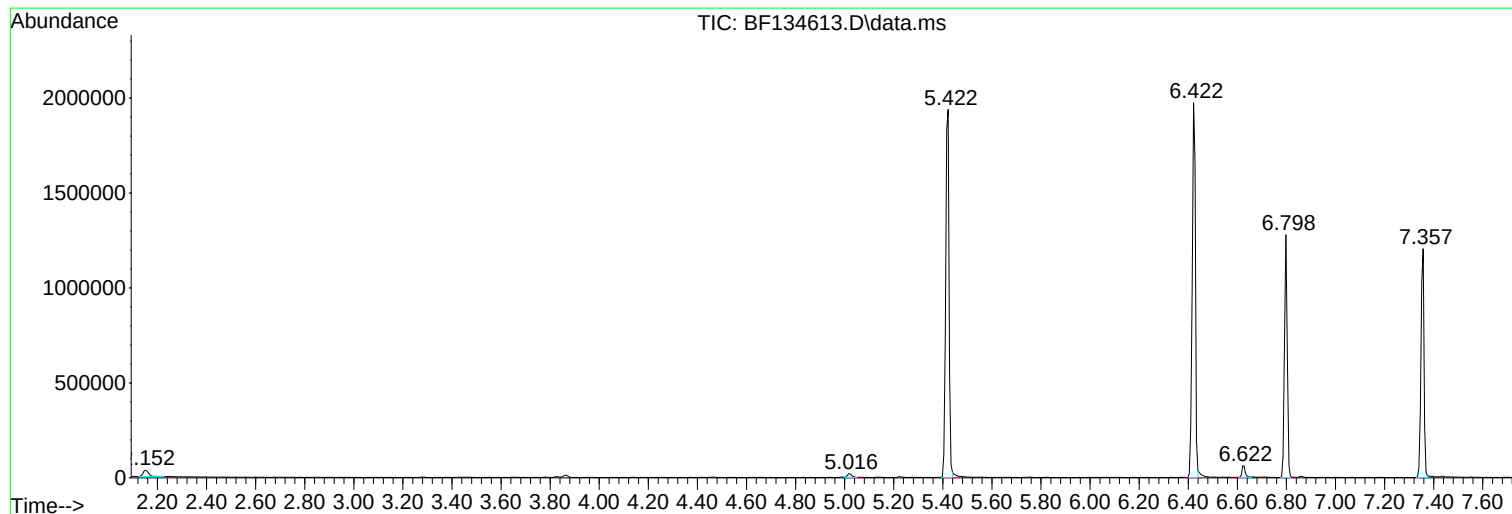

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
Data File : BF134612.D
Acq On : 03 Aug 2023 15:42
Operator : CG\JU
Sample : 03756-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RPTP-9-CS-9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclopentadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.821	6.37 ng	223052	Chrysene-d12	13.968

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentadecane	210	C15H30	000295-48-7	96
2			1-Heneicosyl formate	340	C22H44O2	077899-03-7	95
3			1-Tetracosene	336	C24H48	010192-32-2	95
4			Behenic alcohol	326	C22H46O	000661-19-8	94
5			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	93

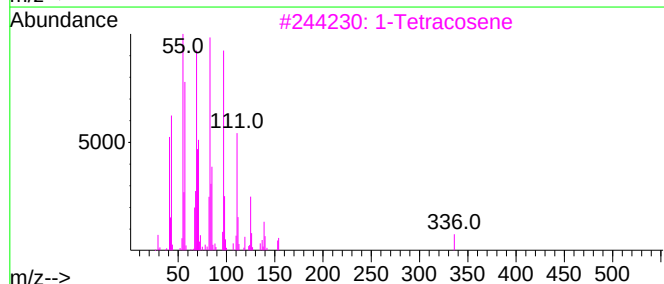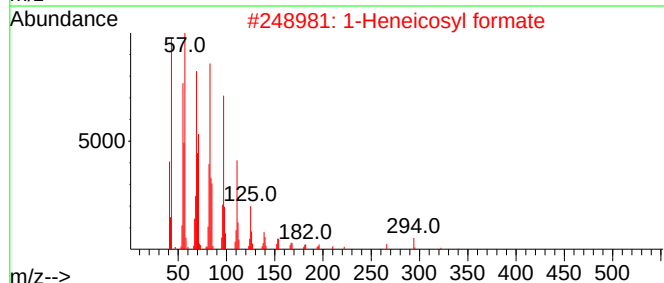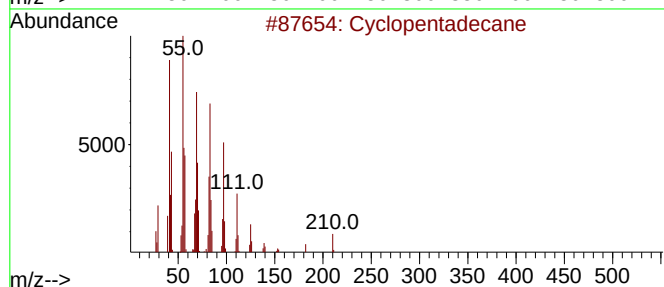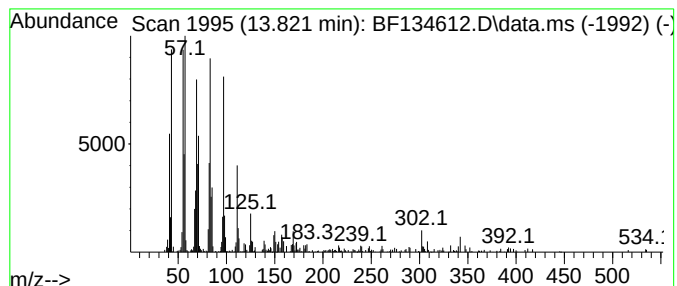

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
Data File : BF134612.D
Acq On : 03 Aug 2023 15:42
Operator : CG\JU
Sample : 03756-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RPTP-9-CS-9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentadecane	13.821	6.4	ng	223052	5	13.968	700179	20.0