
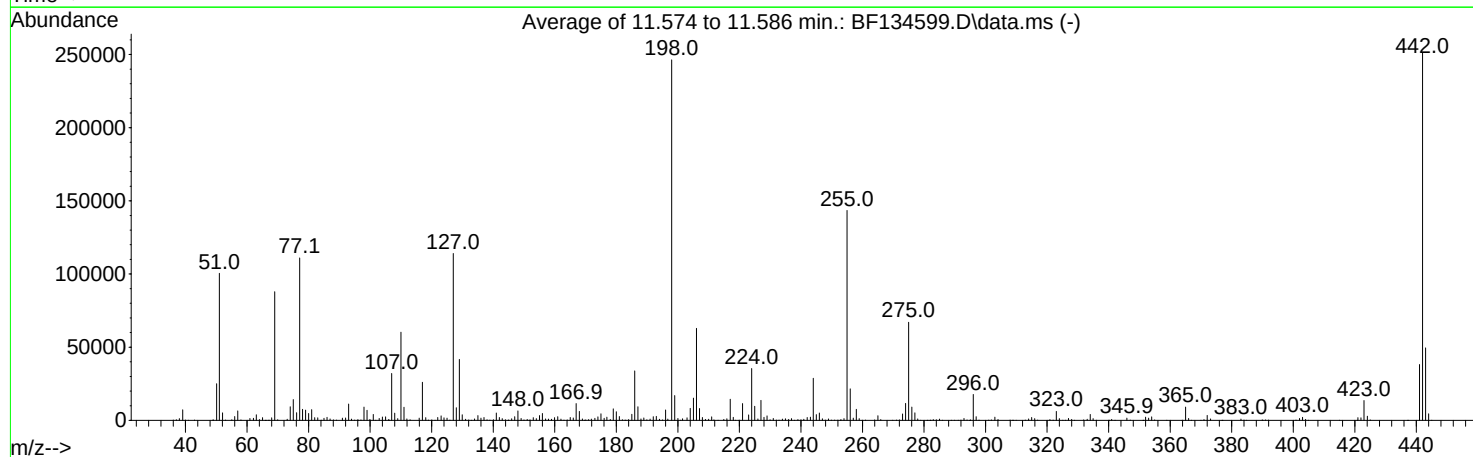


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
 Data File : BF134599.D
 Acq On : 03 Aug 2023 08:13
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 02 02:20:34 2023

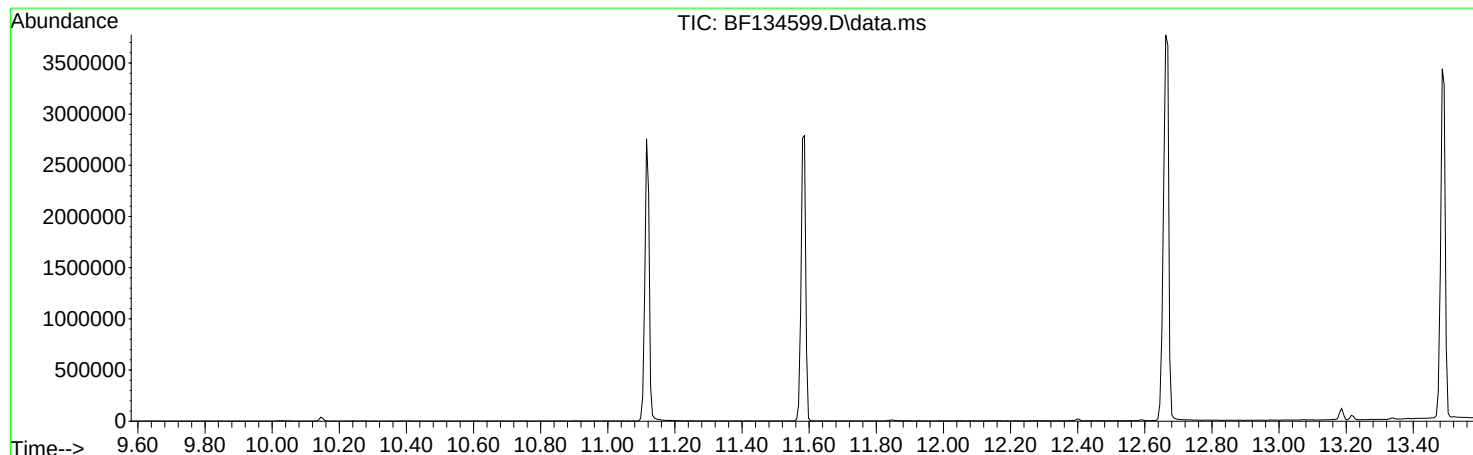




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	100441	PASS
68	69	0.00	2	1.9	1712	PASS
69	198	0.00	100	35.7	87965	PASS
70	69	0.00	2	0.5	474	PASS
127	198	10	80	46.3	114013	PASS
197	198	0.00	2	0.4	904	PASS
198	198	100	100	100.0	246333	PASS
199	198	5	9	6.9	16971	PASS
275	198	10	60	27.2	67061	PASS
365	198	1	100	3.7	9048	PASS
441	198	0.01	100	15.5	38218	PASS
442	442	50	100	100.0	251373	PASS
443	442	15	24	19.7	49556	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
Data File : BF134599.D
Acq On : 03 Aug 2023 08:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 03 14:47:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

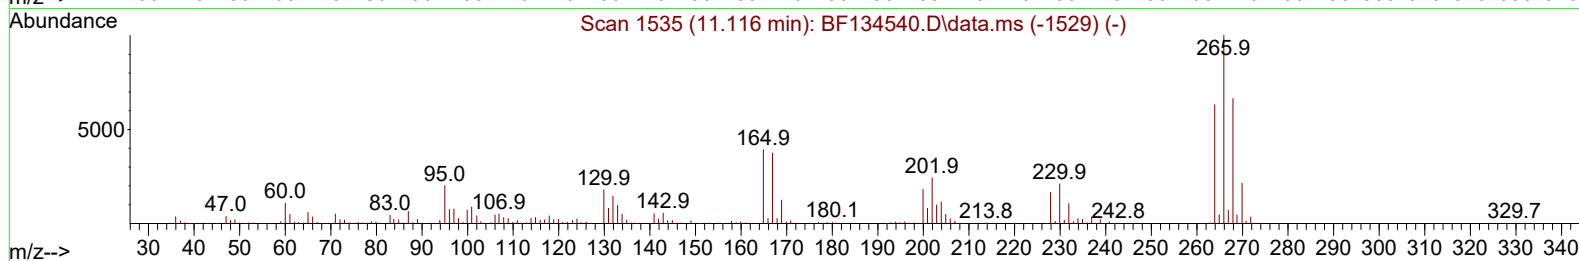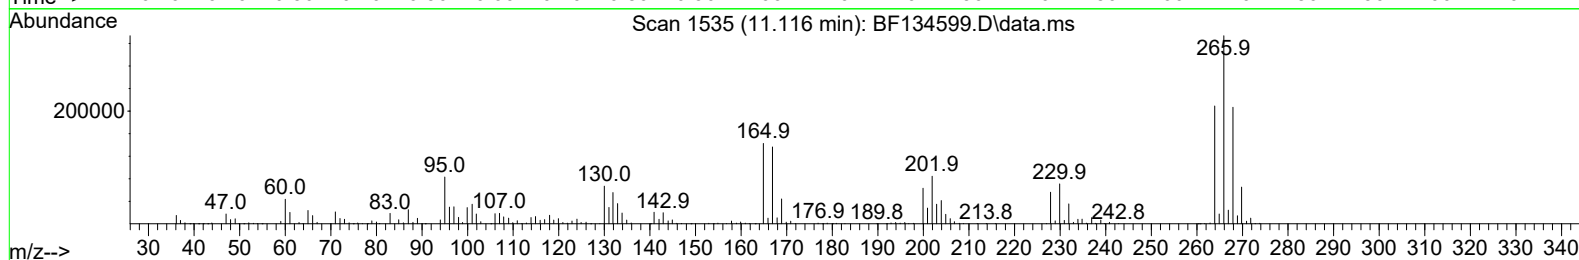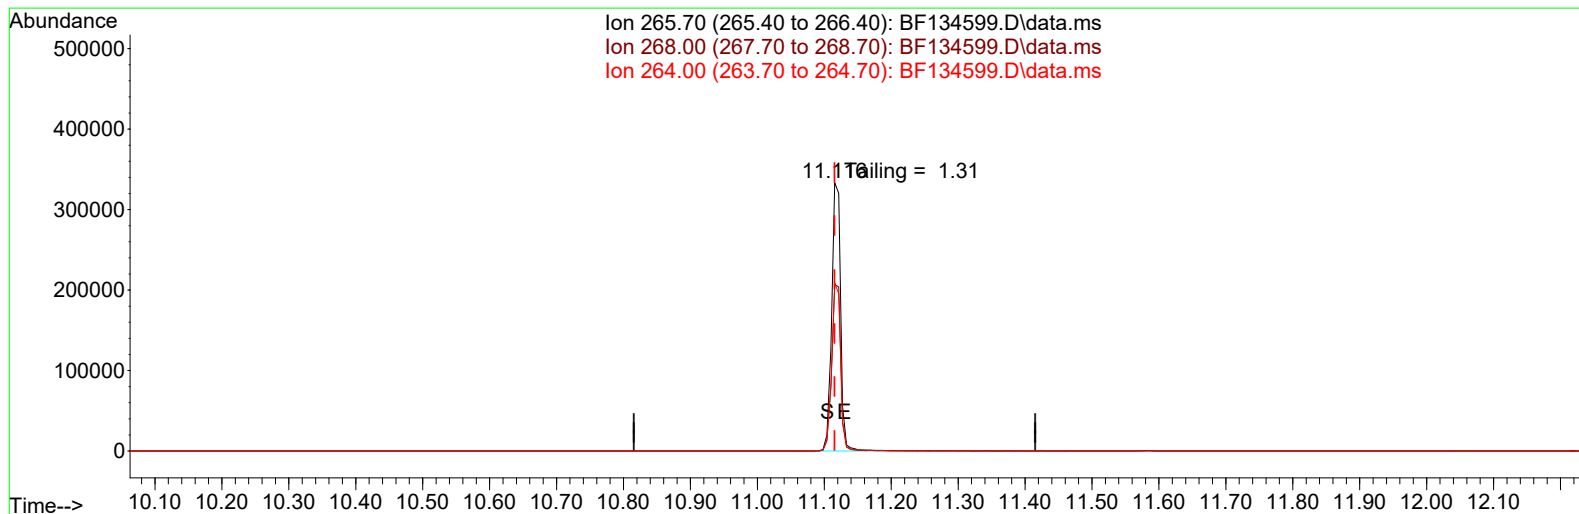

TIC: BF134599.D\data.ms

(70) Pentachlorophenol (C)

11.116min (+ 0.000) 191005.28 ng




response 311697

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.00
264.00	59.70	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080323\
 Data File : BF134599.D
 Acq On : 03 Aug 2023 08:13
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 03 14:47:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 02 02:20:34 2023
 Response via : Initial Calibration

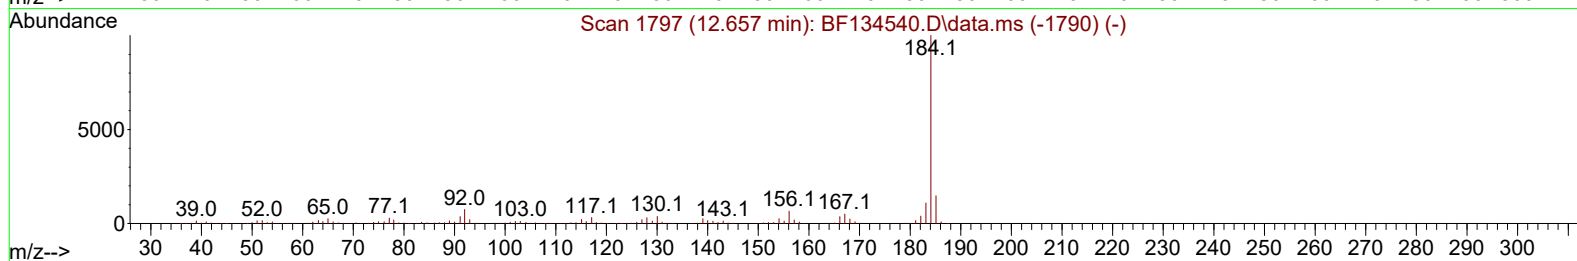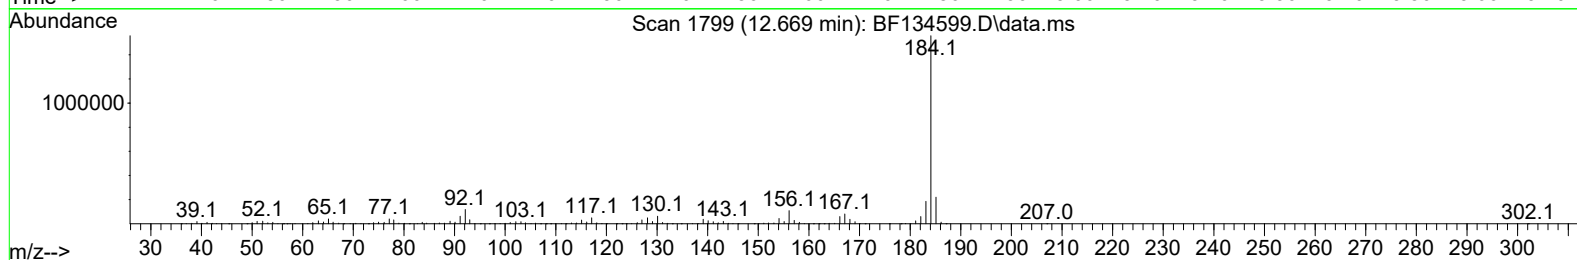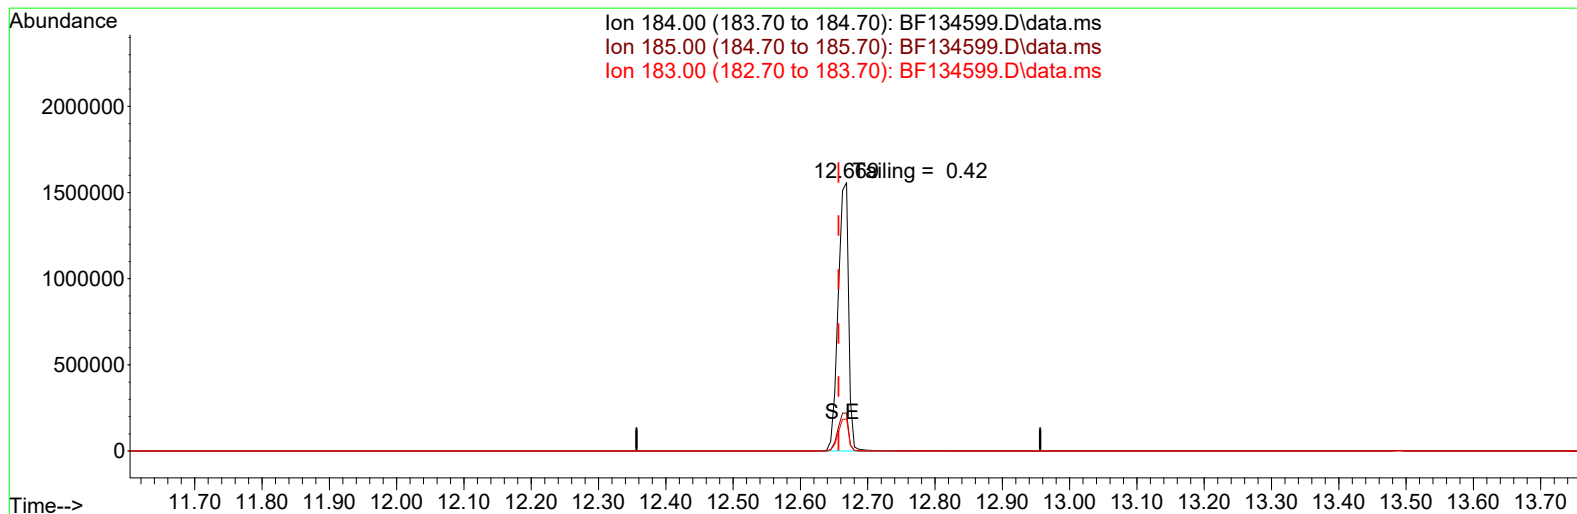

TIC: BF134599.D\data.ms

(77) Benzidine

12.669min (+ 0.012) 588780.03 ng

response 1687114

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.16
183.00	10.80	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2023	BNA_F	<u>BF134599.D</u>
Compound Name	Response	Retention Time
DDT	650317	13.492
DDD	24207	13.186
DDE	265	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24472	674789	3.63

Instrument :
BNA_F
ClientSampleId :
DFTPP