
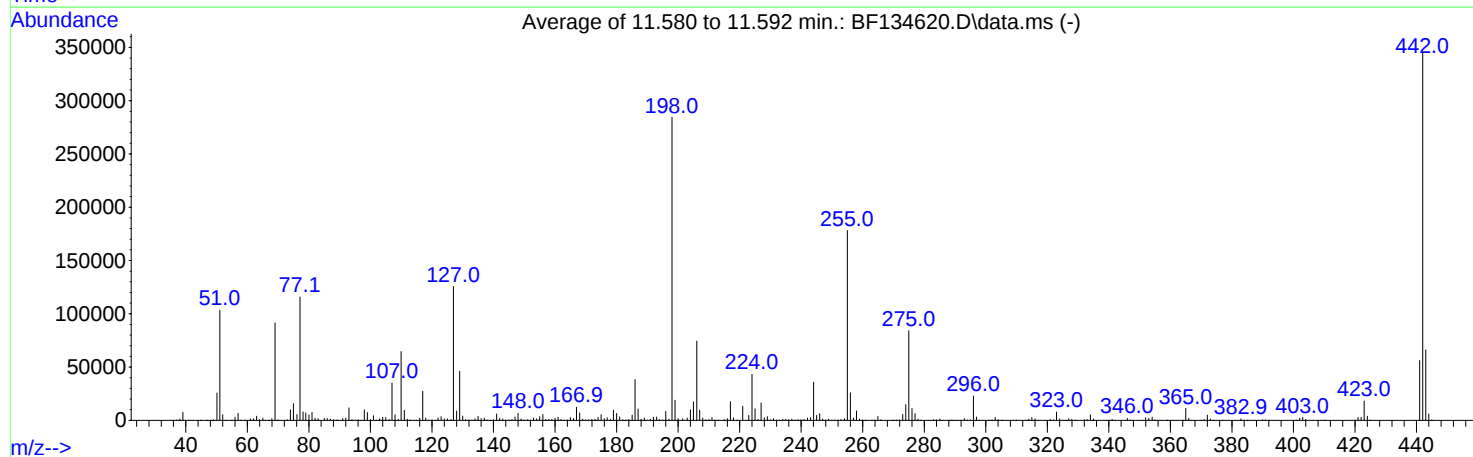


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080423\
 Data File : BF134620.D
 Acq On : 04 Aug 2023 08:28
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 04 09:29:15 2023

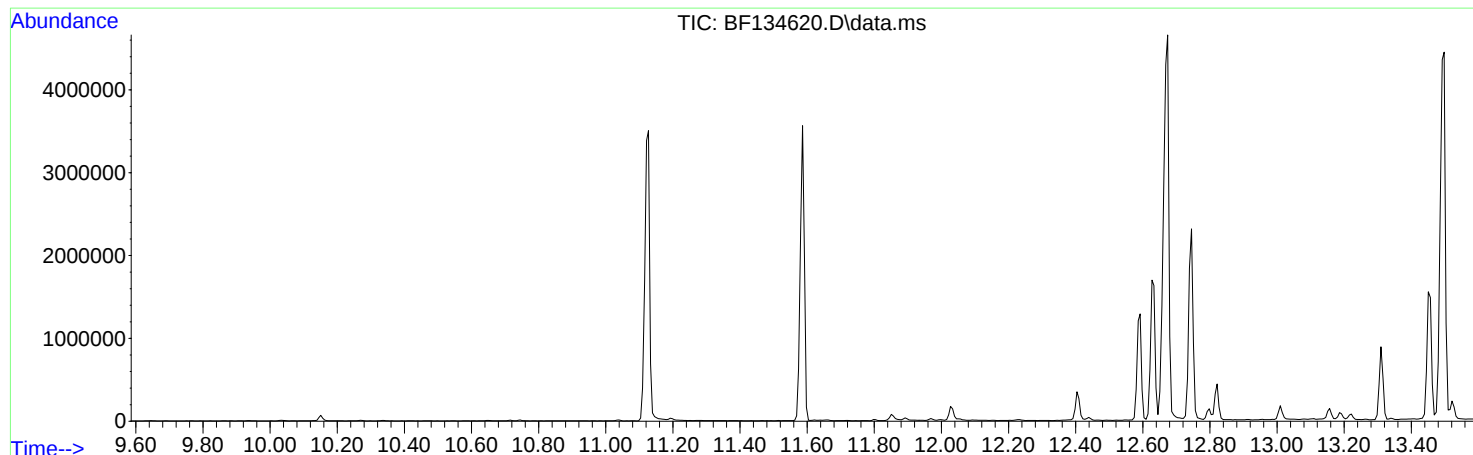




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	103492	PASS
68	69	0.00	2	1.8	1613	PASS
69	198	0.00	100	32.2	91438	PASS
70	69	0.00	2	0.6	525	PASS
127	198	10	80	44.2	125568	PASS
197	198	0.00	2	0.5	1280	PASS
198	198	100	100	100.0	284352	PASS
199	198	5	9	6.7	18915	PASS
275	198	10	60	29.6	84061	PASS
365	198	1	100	4.0	11237	PASS
441	198	0.01	100	19.8	56219	PASS
442	442	50	100	100.0	345216	PASS
443	442	15	24	19.2	66296	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080423\
Data File : BF134620.D
Acq On : 04 Aug 2023 08:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 04 09:34:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

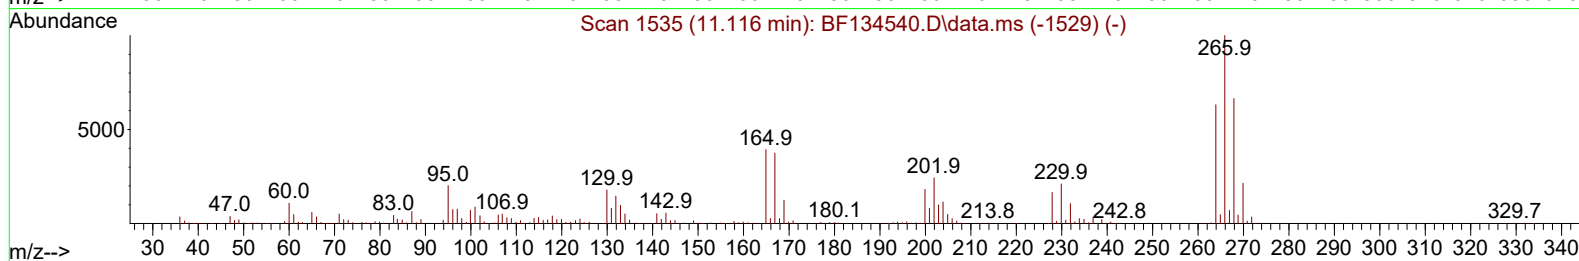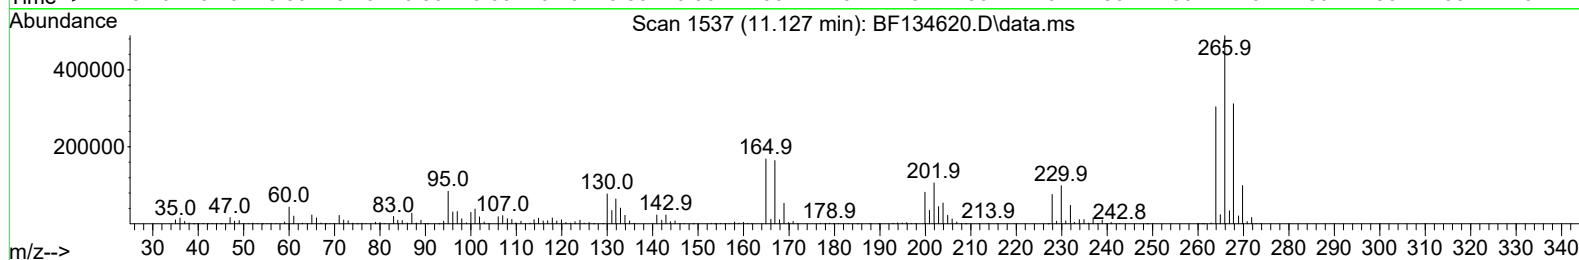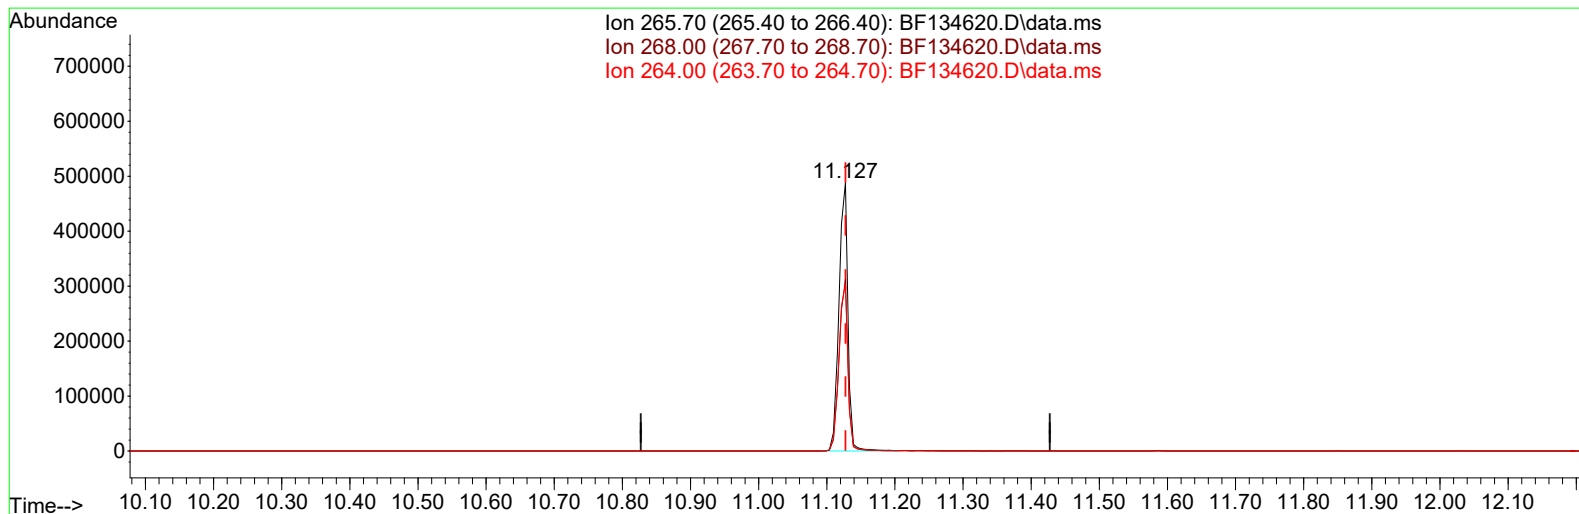

TIC: BF134620.D\data.ms

(70) Pentachlorophenol (C)

11.127min (+ 0.000) 288929.15 ng




response 448749

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.84
264.00	59.70	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080423\
Data File : BF134620.D
Acq On : 04 Aug 2023 08:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 04 09:34:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

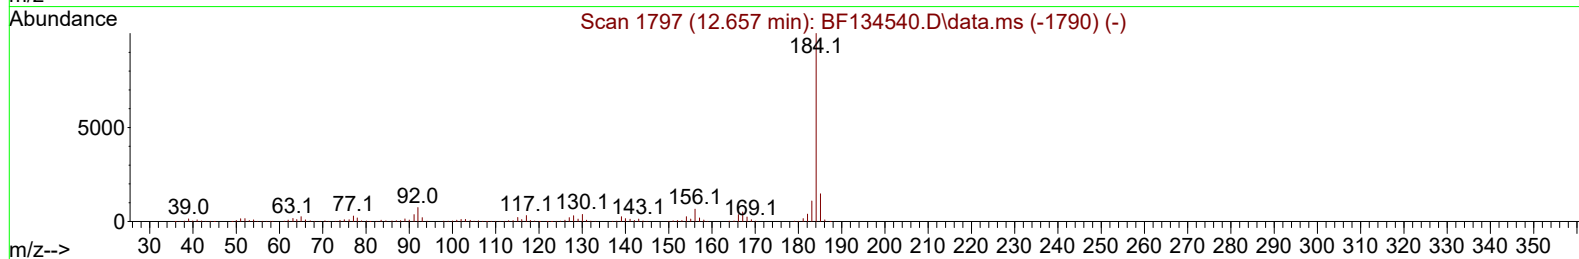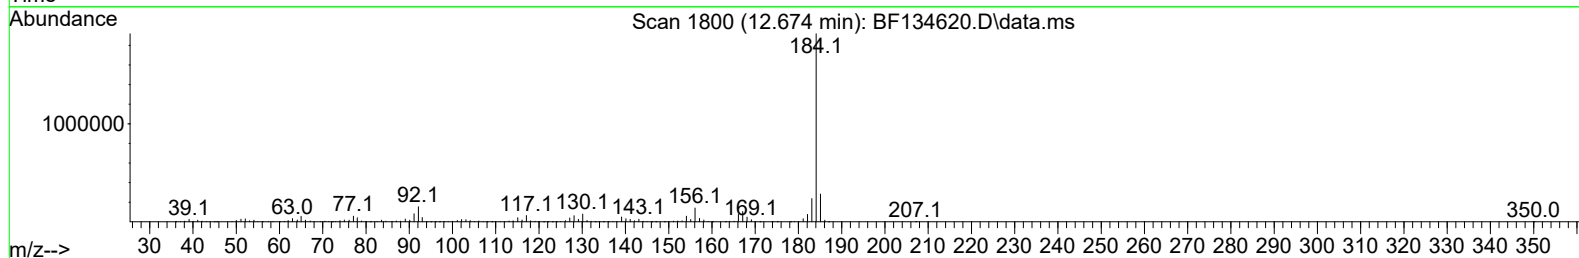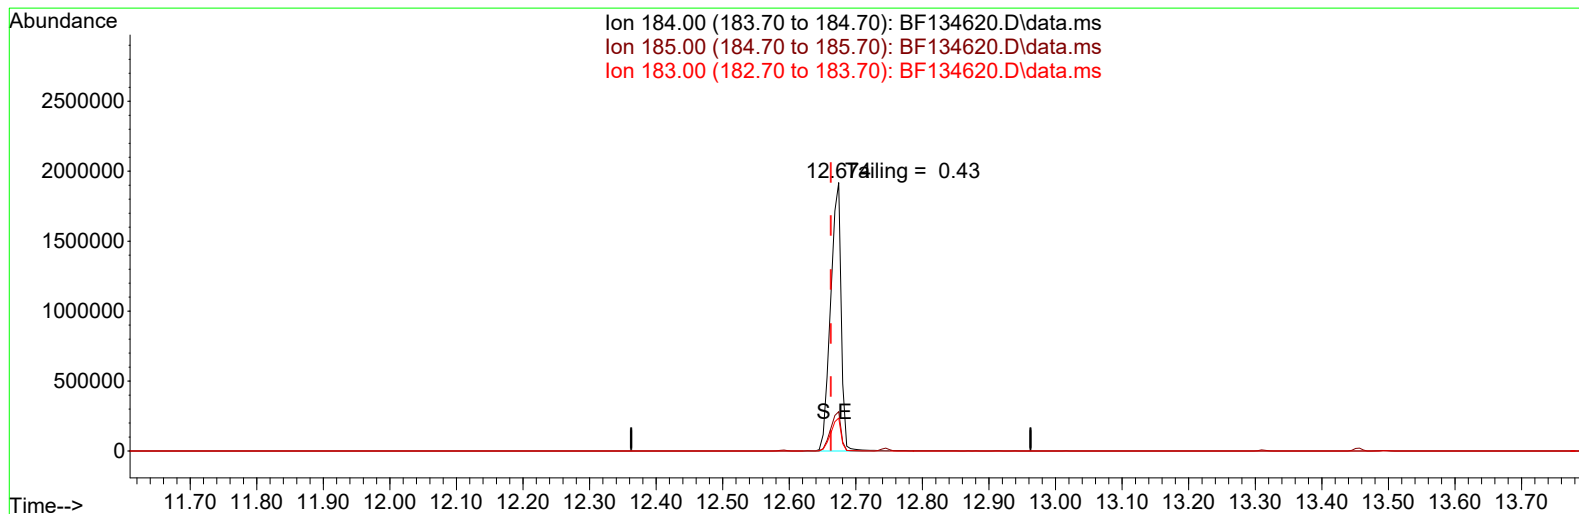

TIC: BF134620.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 299635.68 ng

response 2126957

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.70
183.00	10.80	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2023	BNA_F	<u>BF134620.D</u>
Compound Name	Response	Retention Time
DDT	903204	13.498
DDD	22654	13.186
DDE	384	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23038	926242	2.49

Instrument :
BNA_F
ClientSampleId :
DFTPP