
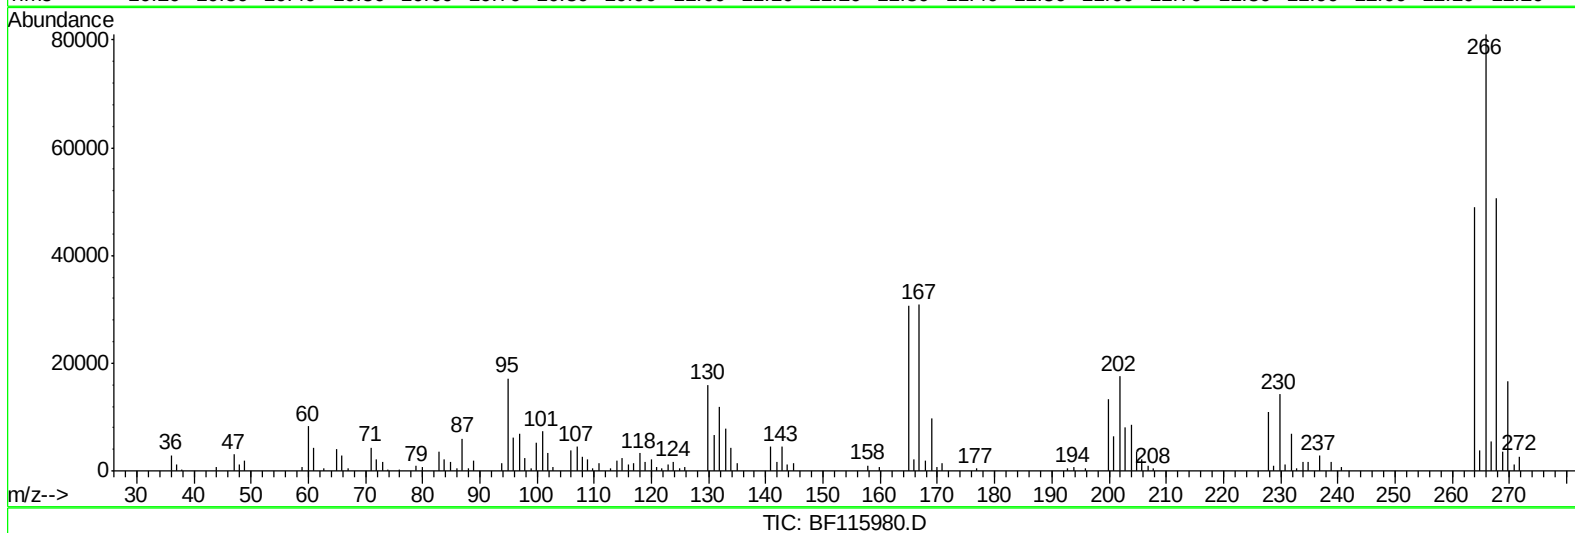


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF080519\
Data File : BF115980.D
Acq On : 5 Aug 2019 13:31
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 09:14:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:31:51 2019
Response via : Initial Calibration

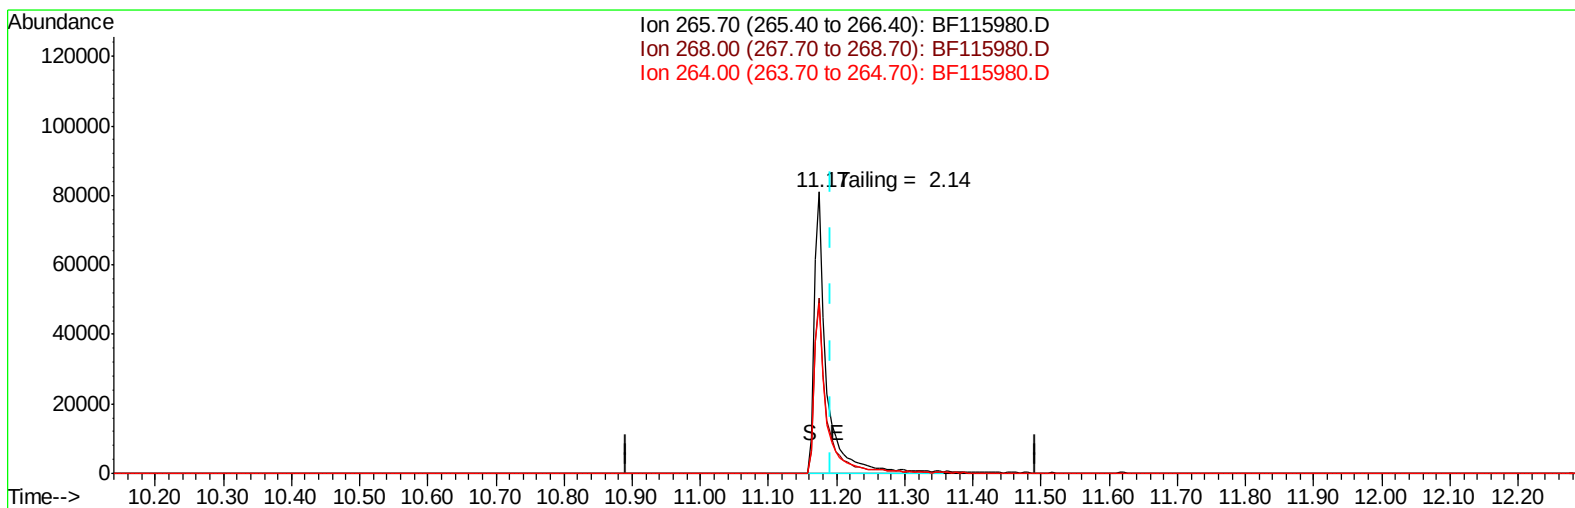

(70) Pentachlorophenol (C)



11.175min (-0.018) 39813.63ng

response 101451

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	62.47
264.00	61.70	60.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF080519\
Data File : BF115980.D
Acq On : 5 Aug 2019 13:31
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 09:14:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:31:51 2019
Response via : Initial Calibration

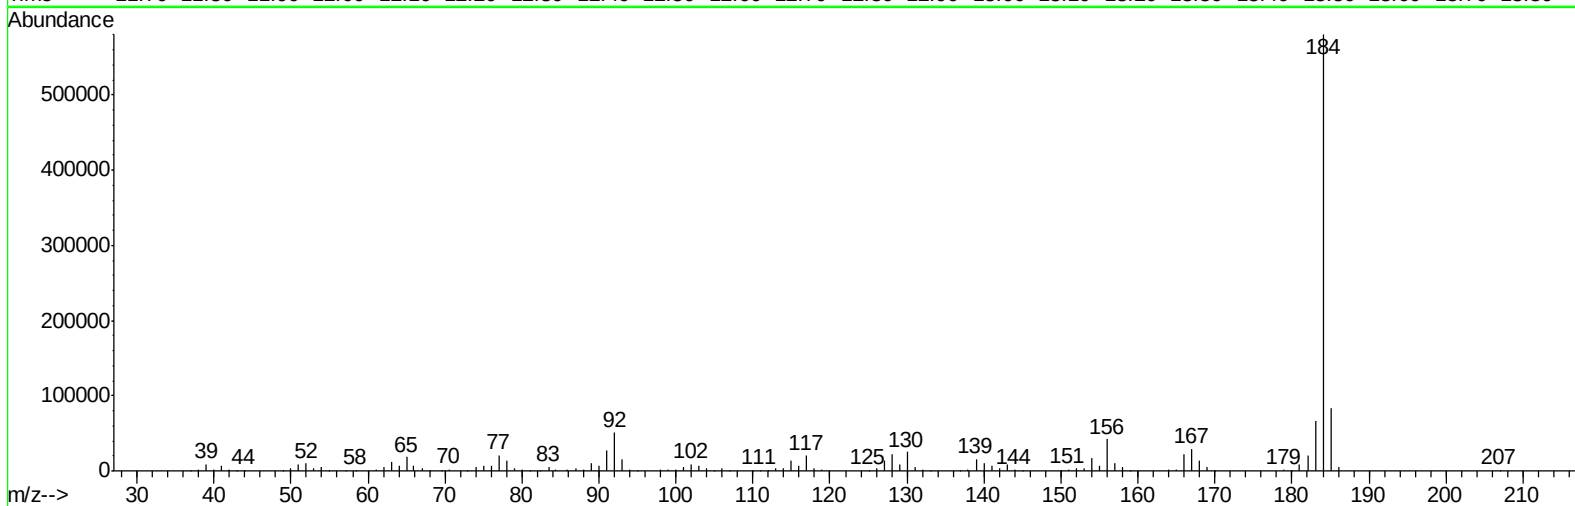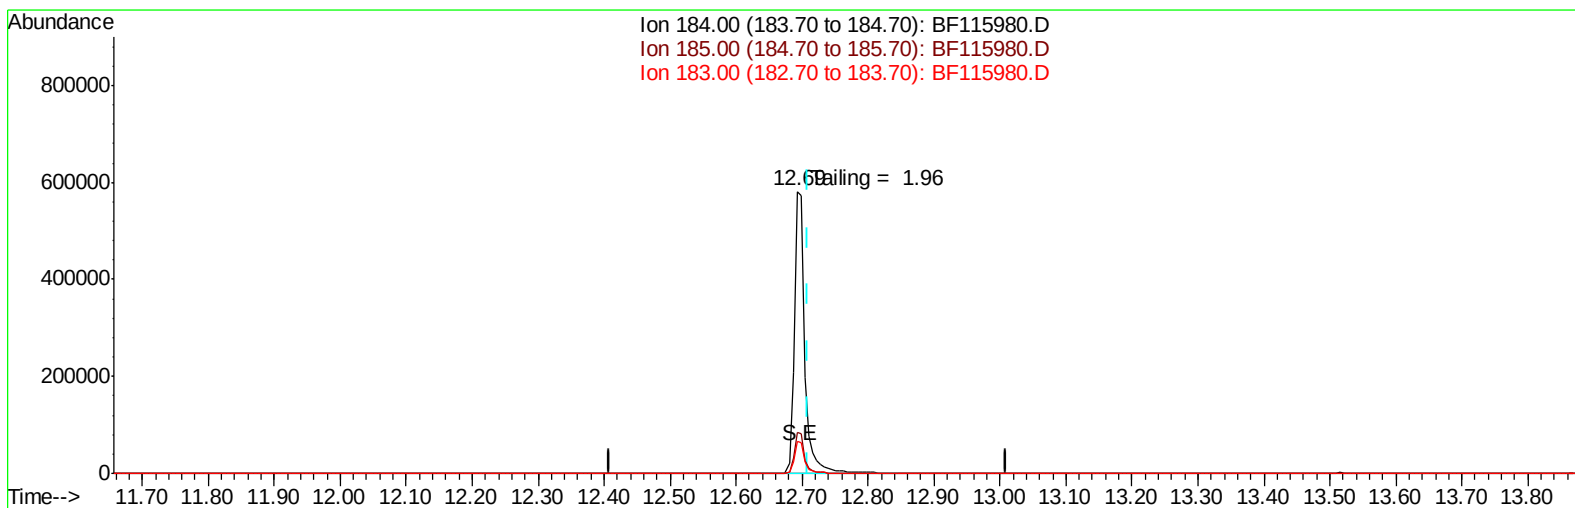

TIC: BF115980.D

(77) Benzidine

12.692min (-0.018) 0.00ng

response 642185

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.48
183.00	11.40	11.42
0.00	0.00	0.00