


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080519\
 Data File : BF115980.D
 Acq On : 5 Aug 2019 13:31
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

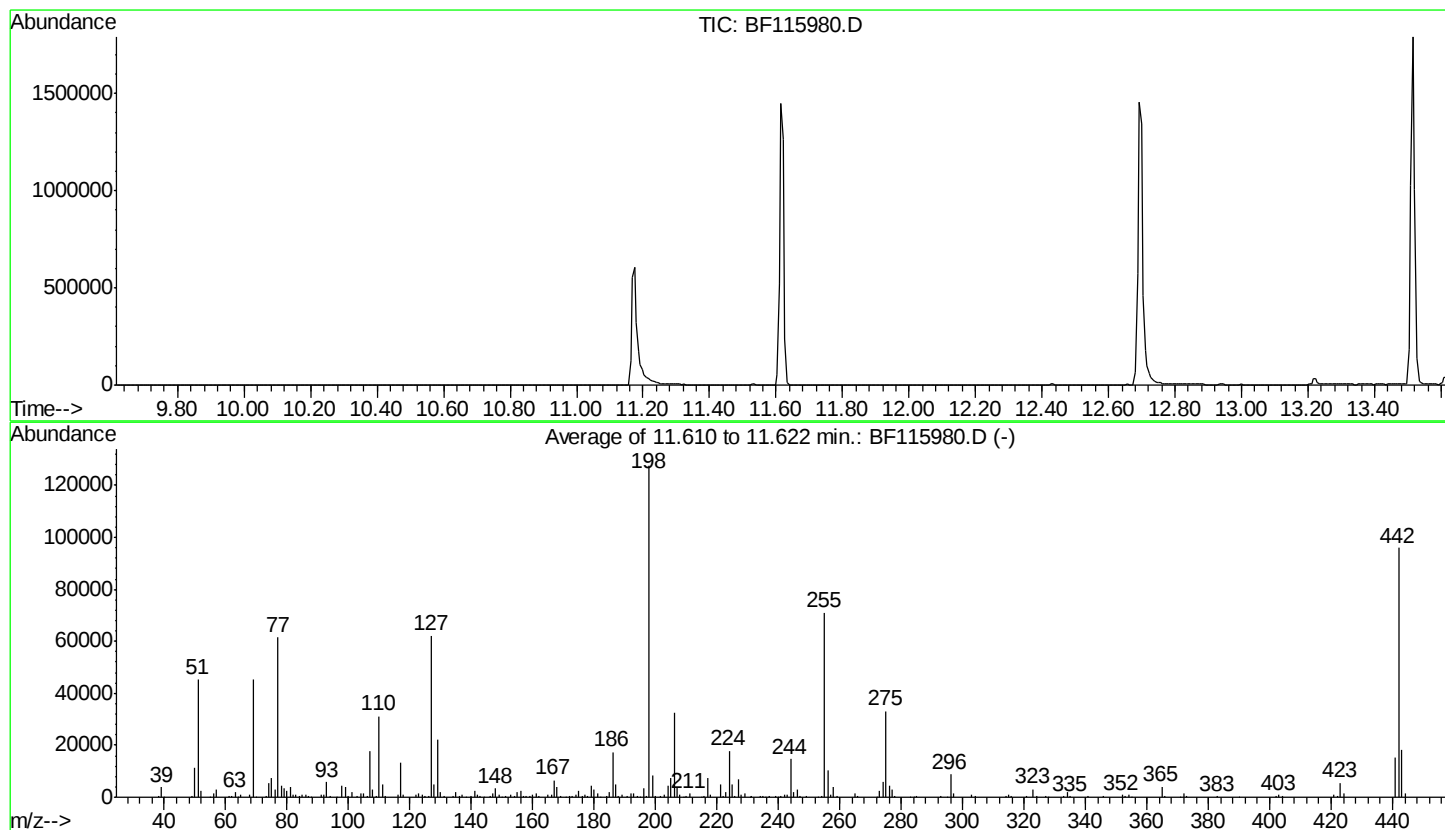

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	45208	PASS
68	69	0.00	2	1.8	816	PASS
69	198	0.00	100	35.5	45354	PASS
70	69	0.00	2	0.3	124	PASS
127	198	10	80	48.8	62320	PASS
197	198	0.00	2	0.5	700	PASS
198	198	100	100	100.0	127613	PASS
199	198	5	9	6.7	8569	PASS
275	198	10	60	26.0	33120	PASS
365	198	1	100	3.2	4105	PASS
441	198	0.01	100	12.0	15264	PASS
442	198	50	100	75.3	96042	PASS
443	442	15	24	19.0	18237	PASS