
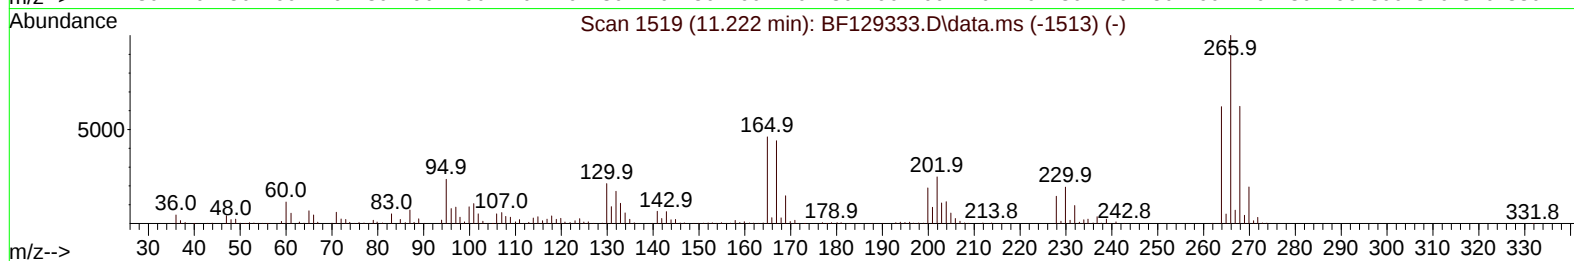
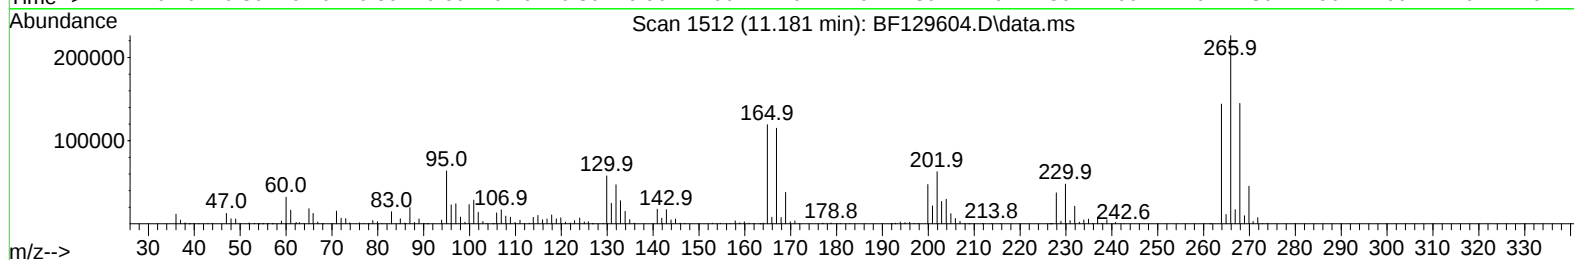


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
Data File : BF129604.D
Acq On : 05 Aug 2022 17:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 04:56:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 16:27:34 2022
Response via : Initial Calibration

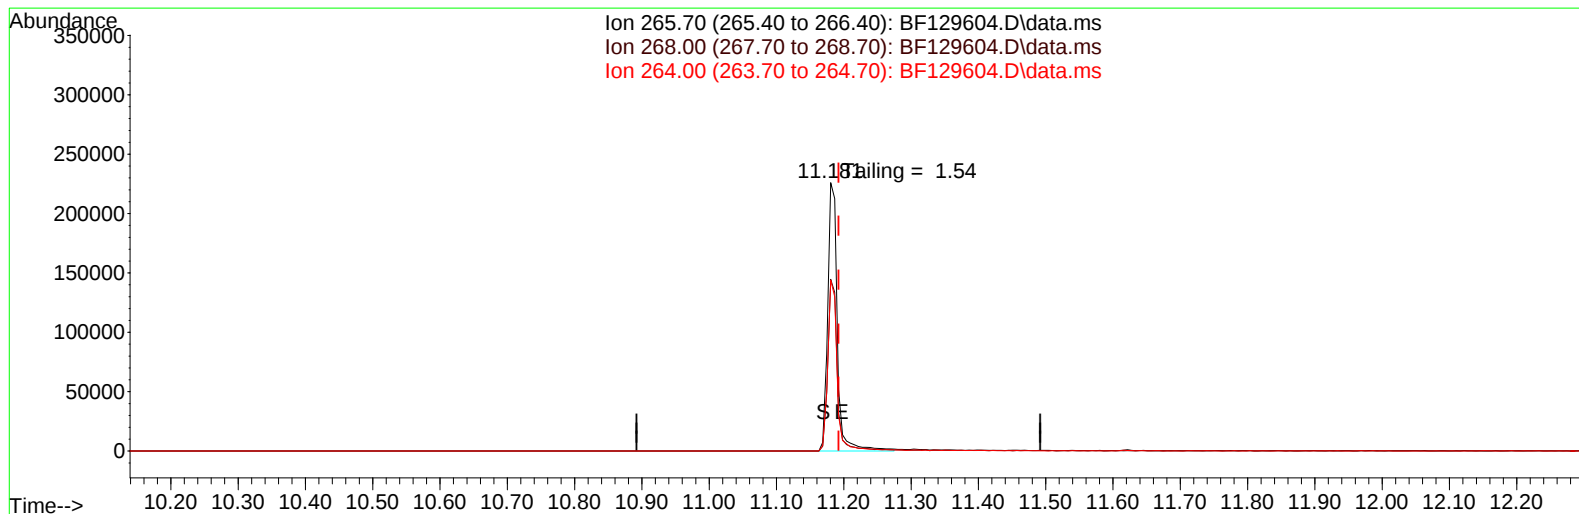

TIC: BF129604.D\data.ms

(70) Pentachlorophenol (C)




11.181min (-0.012) 220925.24 ng

response 226576

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.99
264.00	61.80	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
Data File : BF129604.D
Acq On : 05 Aug 2022 17:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 04:56:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 16:27:34 2022
Response via : Initial Calibration

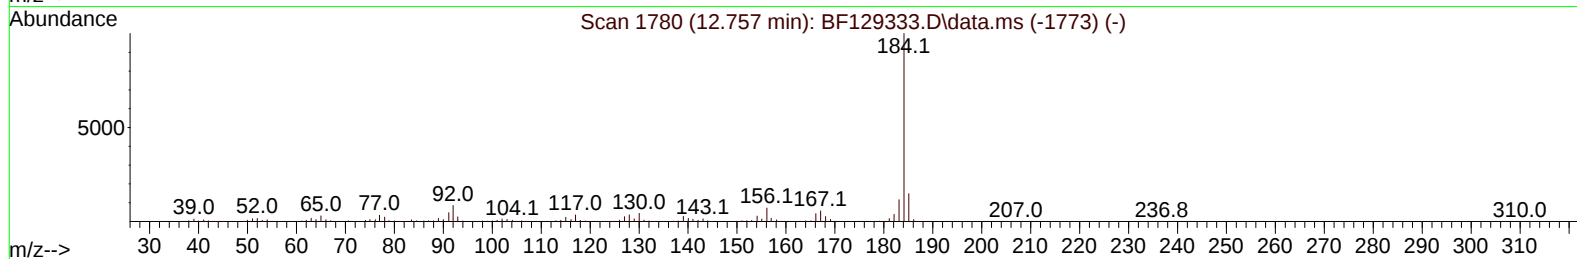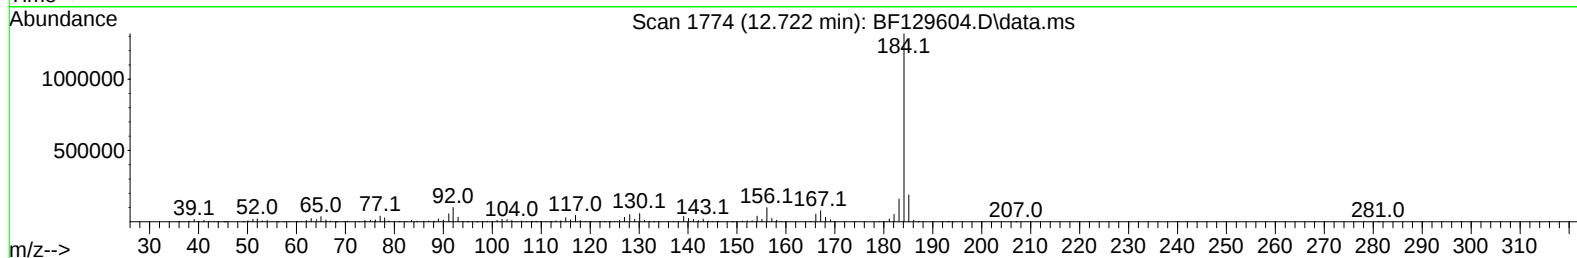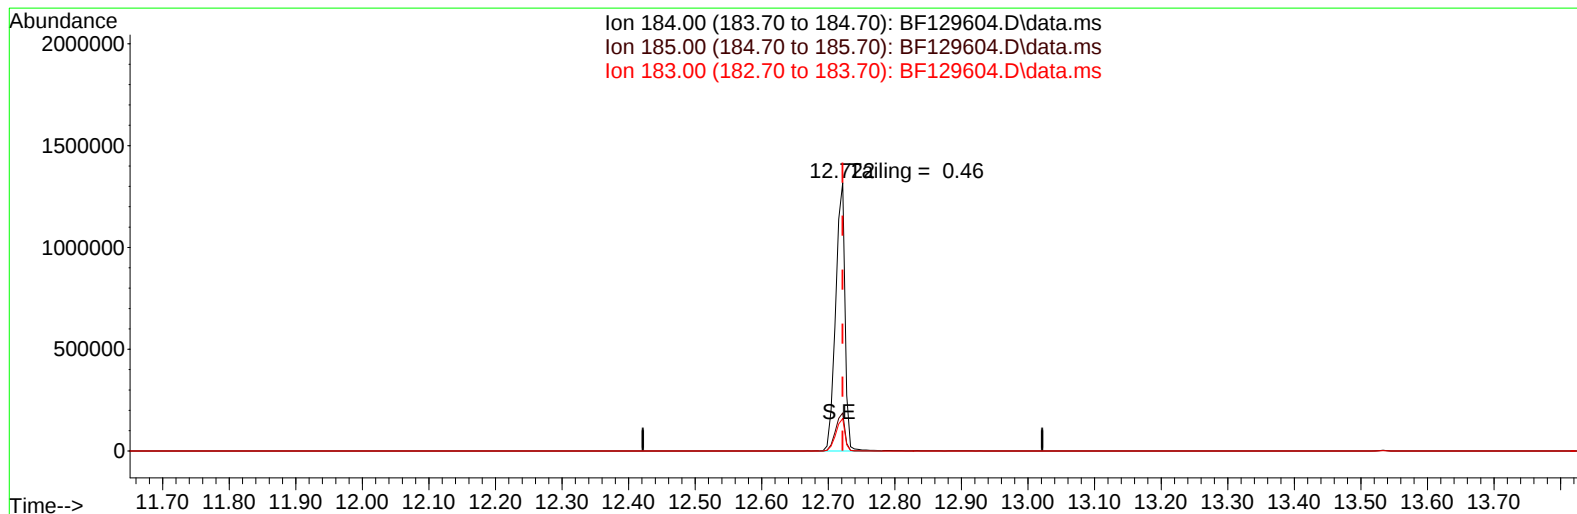

TIC: BF129604.D\data.ms

(77) Benzidine

12.722min (+ 0.000) 25870.47 ng

response 1282257

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.23
183.00	11.60	12.09
0.00	0.00	0.00