

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
 Data File : BF129595.D
 Acq On : 05 Aug 2022 11:31
 Operator : CG\JU
 Sample : PB146609BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146609BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129595.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	540	545	548	rBV	4958693	4802561	76.25%	12.552%
2	6.498	711	716	719	rBV	4396297	4910518	77.96%	12.834%
3	6.845	772	775	779	rVB	1263675	1049115	16.66%	2.742%
4	7.416	866	872	875	rBV	3115761	3247274	51.55%	8.487%
5	8.134	988	994	997	rBV	1537870	1472740	23.38%	3.849%
6	9.210	1170	1177	1180	rBV	6140034	6077029	96.48%	15.883%
7	9.886	1287	1292	1296	rBV	2010266	1720035	27.31%	4.496%
8	10.686	1421	1428	1431	rBV	3926337	3966827	62.98%	10.368%
9	11.380	1540	1546	1549	rBV	1884469	1729458	27.46%	4.520%
10	12.969	1810	1816	1819	rBV	6450559	6298786	100.00%	16.463%
11	14.021	1991	1995	1999	rBV	1639924	1396980	22.18%	3.651%
12	14.110	2004	2010	2016	rBV	365069	405944	6.44%	1.061%
13	15.498	2241	2246	2256	rVB	965078	1183954	18.80%	3.094%




Sum of corrected areas: 38261221

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
Data File : BF129595.D
Acq On : 05 Aug 2022 11:31
Operator : CG\JU
Sample : PB146609BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146609BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

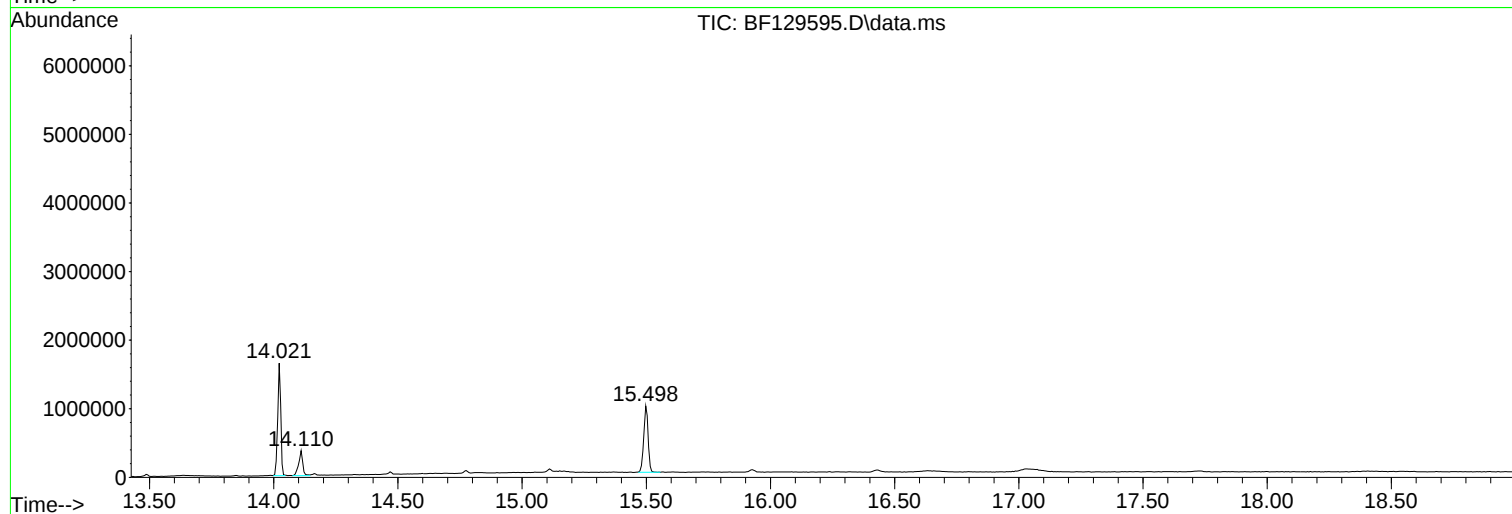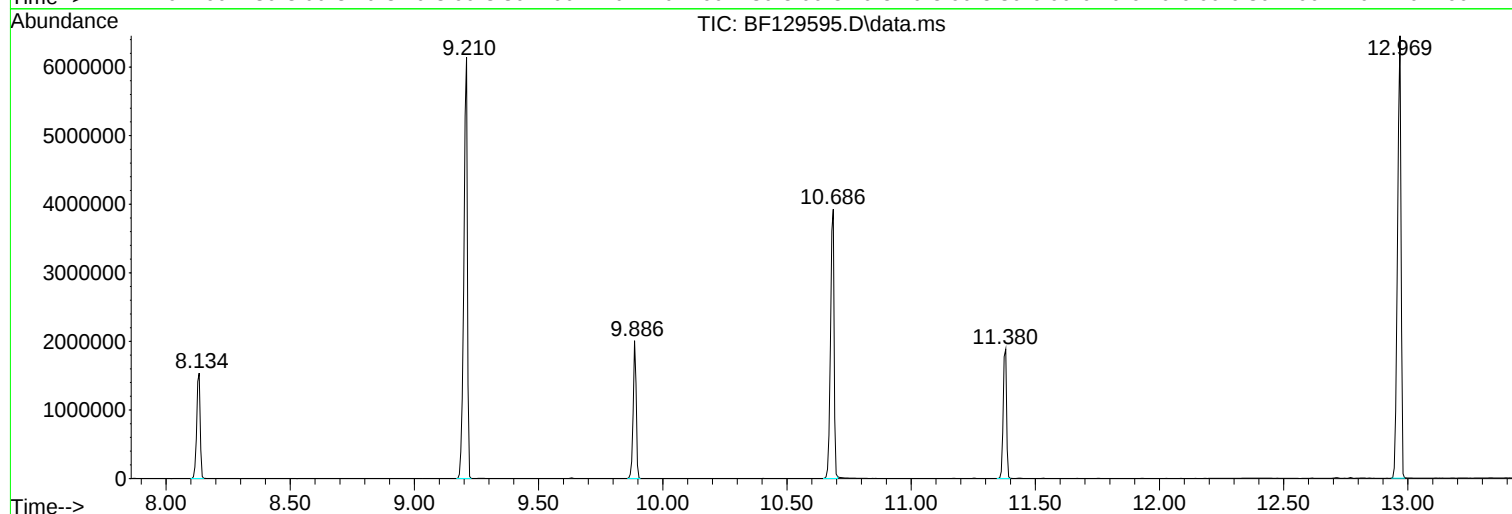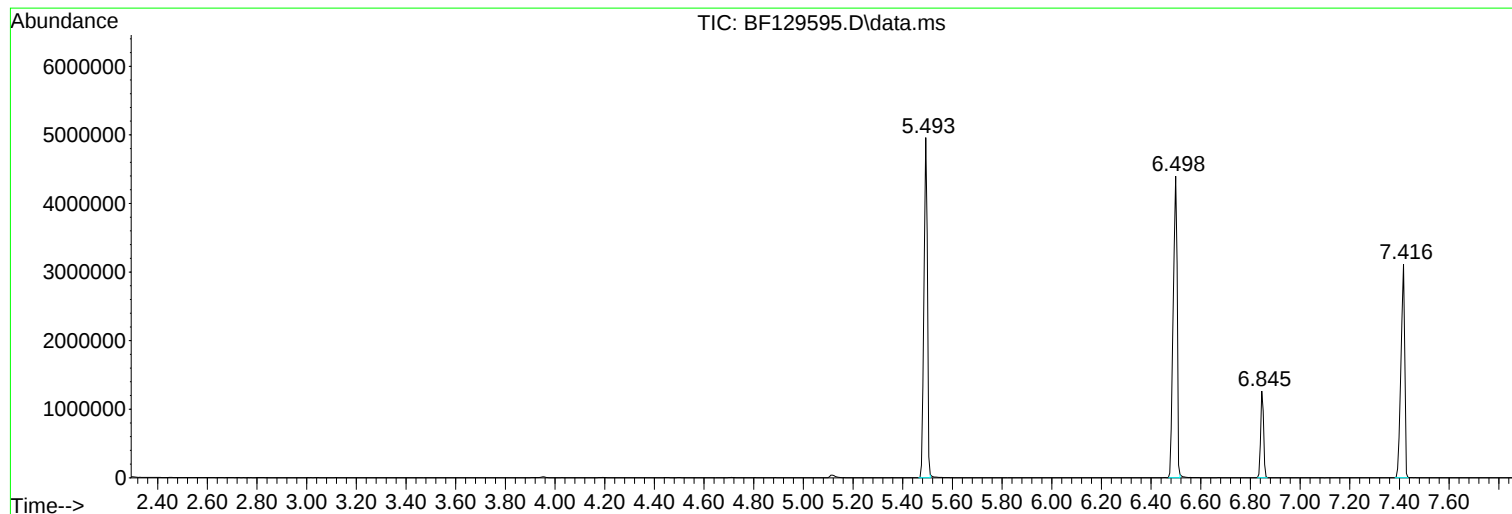

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
Data File : BF129595.D
Acq On : 05 Aug 2022 11:31
Operator : CG\JU
Sample : PB146609BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146609BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.110	5.81 ng	405944	Chrysene-d12	14.022

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	76
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	64
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	38
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	28

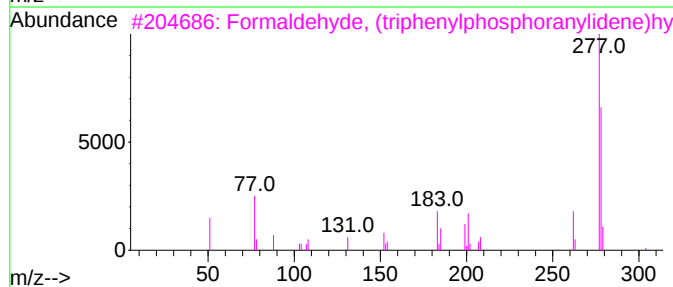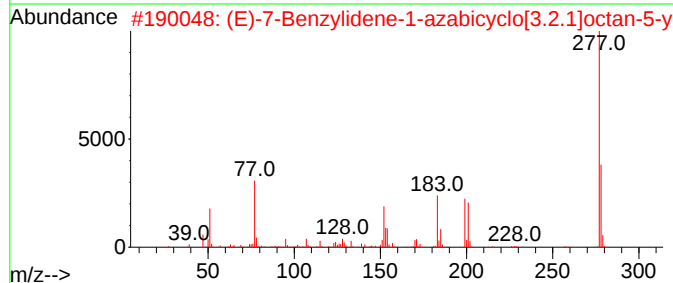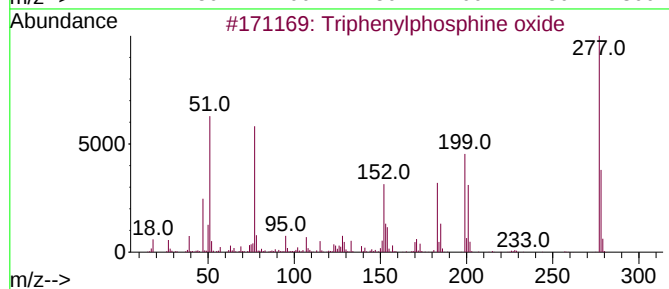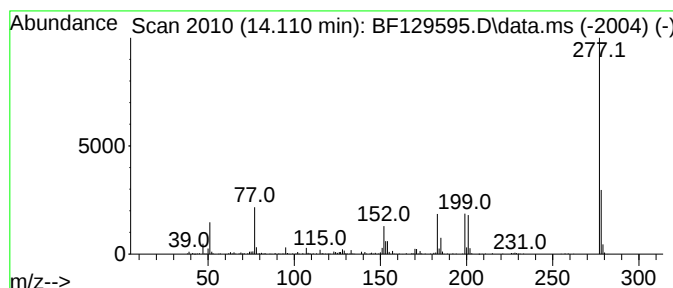

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
Data File : BF129595.D
Acq On : 05 Aug 2022 11:31
Operator : CG\JU
Sample : PB146609BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146609BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.110	5.8	ng	405944	5	14.022	1396980	20.0