

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
 Data File : BF129621.D
 Acq On : 06 Aug 2022 02:53
 Operator : CG\JU
 Sample : N4061-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP1-0804

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129621.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.910	271	276	282	rVB	122907	167571	6.85%	0.707%
2	5.434	532	535	537	rBV	36445	41849	1.71%	0.177%
3	5.487	540	544	559	rVB	2667420	2445792	100.00%	10.323%
4	6.451	705	708	711	rBV	57638	46258	1.89%	0.195%
5	6.504	713	717	727	rVB	2398913	2296655	93.90%	9.693%
6	6.845	772	775	782	rBV	1009462	841862	34.42%	3.553%
7	6.916	782	787	791	rBV4	26485	49522	2.02%	0.209%
8	7.110	815	820	826	rBV2	46683	56778	2.32%	0.240%
9	7.275	843	848	853	rVB2	107694	115504	4.72%	0.487%
10	7.410	867	871	874	rBV	1665765	1399098	57.20%	5.905%
11	7.581	898	900	904	rVB	125701	103395	4.23%	0.436%
12	8.128	990	993	996	rBV	1165281	968865	39.61%	4.089%
13	8.181	999	1002	1004	rVB	48831	45368	1.85%	0.191%
14	8.410	1038	1041	1046	rVB3	50219	60083	2.46%	0.254%
15	8.628	1075	1078	1080	rBV	59967	46893	1.92%	0.198%
16	8.839	1111	1114	1117	rBV	65173	69354	2.84%	0.293%
17	8.904	1121	1125	1127	rBV4	48681	59204	2.42%	0.250%
18	9.139	1163	1165	1172	rVB5	55400	56771	2.32%	0.240%
19	9.204	1172	1176	1179	rBV	2706856	2215338	90.58%	9.350%
20	9.275	1184	1188	1191	rBV2	101611	121256	4.96%	0.512%
21	9.310	1191	1194	1197	rBV4	41086	58055	2.37%	0.245%
22	9.463	1218	1220	1225	rVB2	36070	44535	1.82%	0.188%
23	9.539	1230	1233	1236	rVV3	102247	113741	4.65%	0.480%
24	9.586	1238	1241	1245	rVB3	147628	173818	7.11%	0.734%
25	9.745	1265	1268	1270	rBV	184709	162290	6.64%	0.685%
26	9.786	1273	1275	1280	rVB3	112791	126039	5.15%	0.532%
27	9.886	1289	1292	1294	rVB	1097148	869988	35.57%	3.672%
28	9.916	1294	1297	1305	rVB	260297	293595	12.00%	1.239%
29	10.086	1324	1326	1331	rVB	102623	107080	4.38%	0.452%
30	10.216	1342	1348	1351	rBV6	117568	231775	9.48%	0.978%
31	10.286	1357	1360	1365	rBV4	161080	195085	7.98%	0.823%
32	10.404	1377	1380	1383	rBV	456313	393767	16.10%	1.662%
33	10.433	1383	1385	1387	rVB	109955	86350	3.53%	0.364%
34	10.680	1423	1427	1430	rBV	1477206	1321437	54.03%	5.577%
35	10.792	1443	1446	1447	rBV	241491	234825	9.60%	0.991%
36	10.857	1454	1457	1459	rBV	320155	329005	13.45%	1.389%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
Data File : BF129621.D
Acq On : 06 Aug 2022 02:53
Operator : CG\JU
Sample : N4061-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP1-0804

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	10.886	1460	1462	1466	rVV2	266413	303595	12.41%	1.281%
38	10.922	1466	1468	1470	rBV	312935	236592	9.67%	0.999%
39	10.975	1475	1477	1478	rBV2	129879	106150	4.34%	0.448%
40	11.033	1485	1487	1490	rVB3	278806	261507	10.69%	1.104%
41	11.069	1491	1493	1496	rBV	213255	204650	8.37%	0.864%
42	11.375	1542	1545	1548	rBV	947322	985175	40.28%	4.158%
43	11.398	1548	1549	1555	rVB	610938	513827	21.01%	2.169%
44	11.451	1556	1558	1560	rBV	198954	164472	6.72%	0.694%
45	12.486	1732	1734	1738	rVB	634545	541720	22.15%	2.286%
46	12.598	1750	1753	1756	rBV	1390852	1194888	48.85%	5.043%
47	12.827	1790	1792	1794	rBV	939193	673388	27.53%	2.842%
48	12.963	1812	1815	1822	rVB	1931590	1851157	75.69%	7.813%
49	13.992	1988	1990	1993	rBV	827529	707598	28.93%	2.986%




Sum of corrected areas: 23693520

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
Data File : BF129621.D
Acq On : 06 Aug 2022 02:53
Operator : CG\JU
Sample : N4061-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP1-0804

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

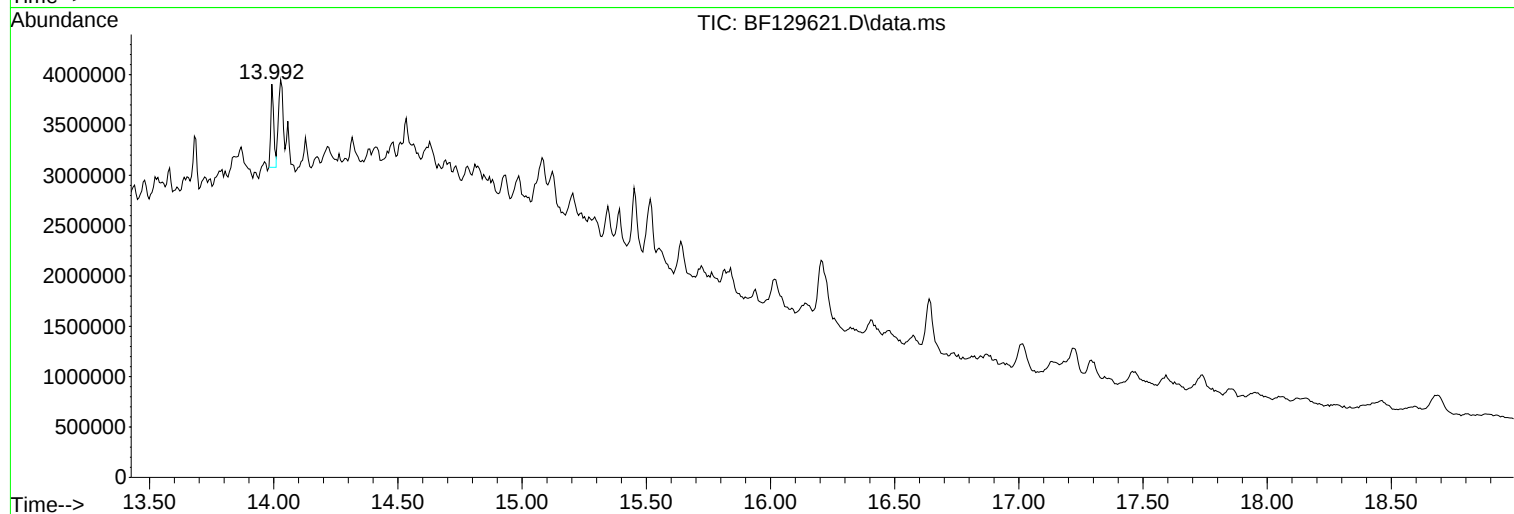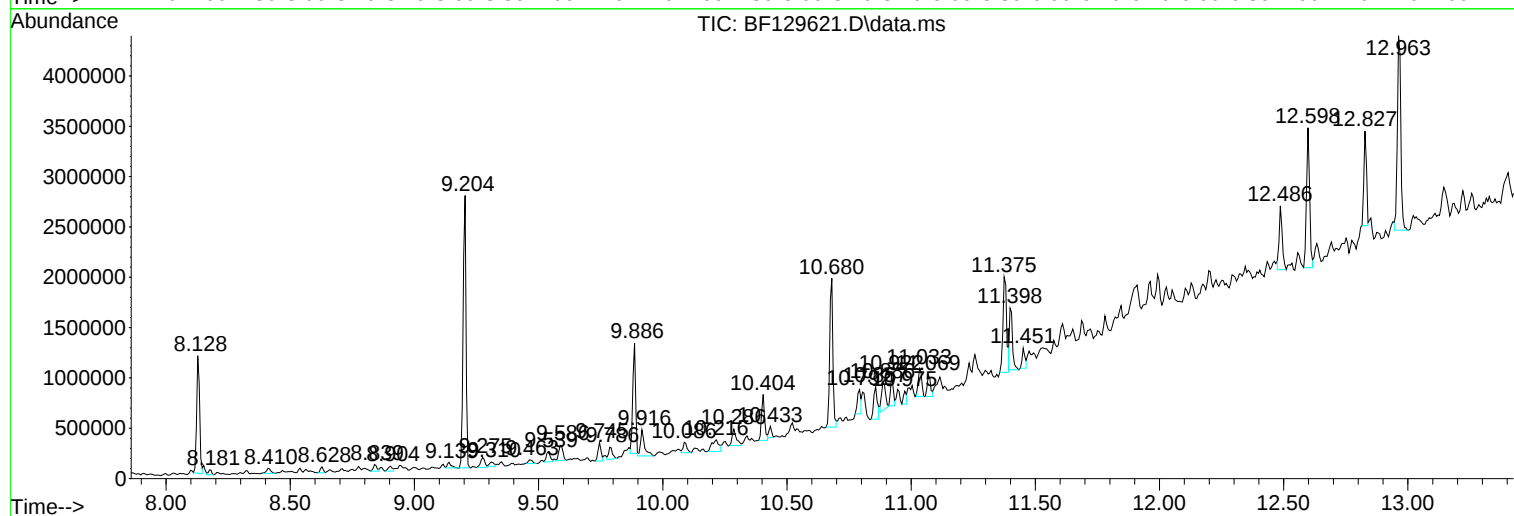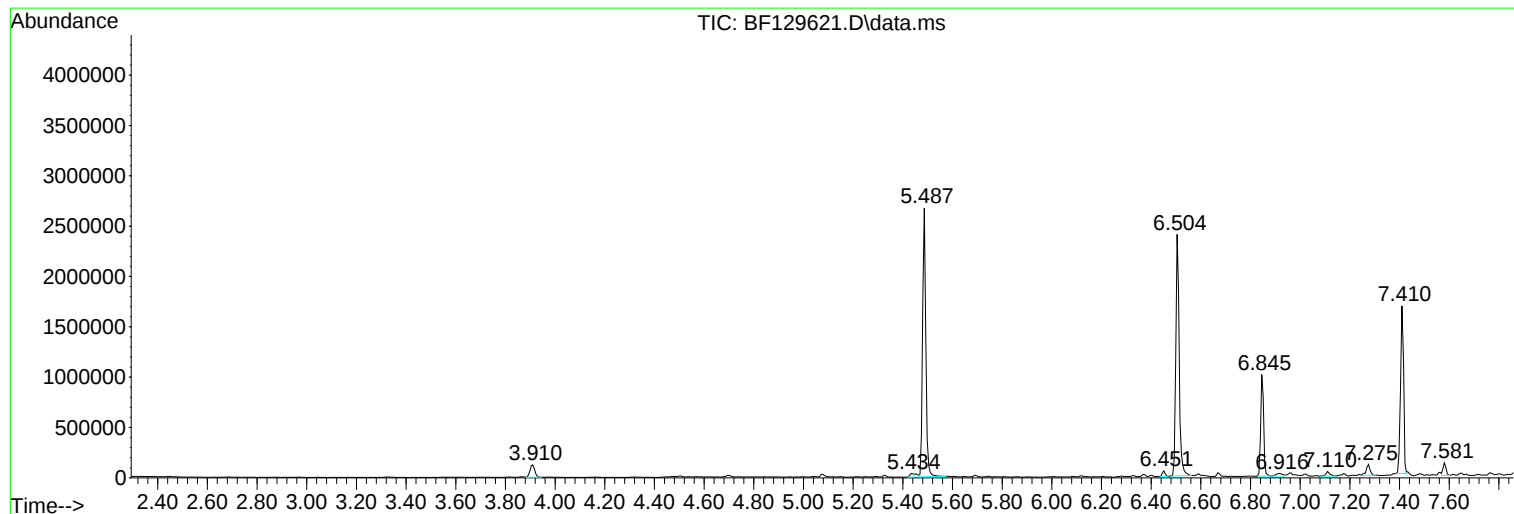

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
Data File : BF129621.D
Acq On : 06 Aug 2022 02:53
Operator : CG\JU
Sample : N4061-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP1-0804

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
Data File : BF129621.D
Acq On : 06 Aug 2022 02:53
Operator : CG\JU
Sample : N4061-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP1-0804

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------