


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
 Data File : BF129593.D
 Acq On : 05 Aug 2022 10:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 05 16:27:34 2022

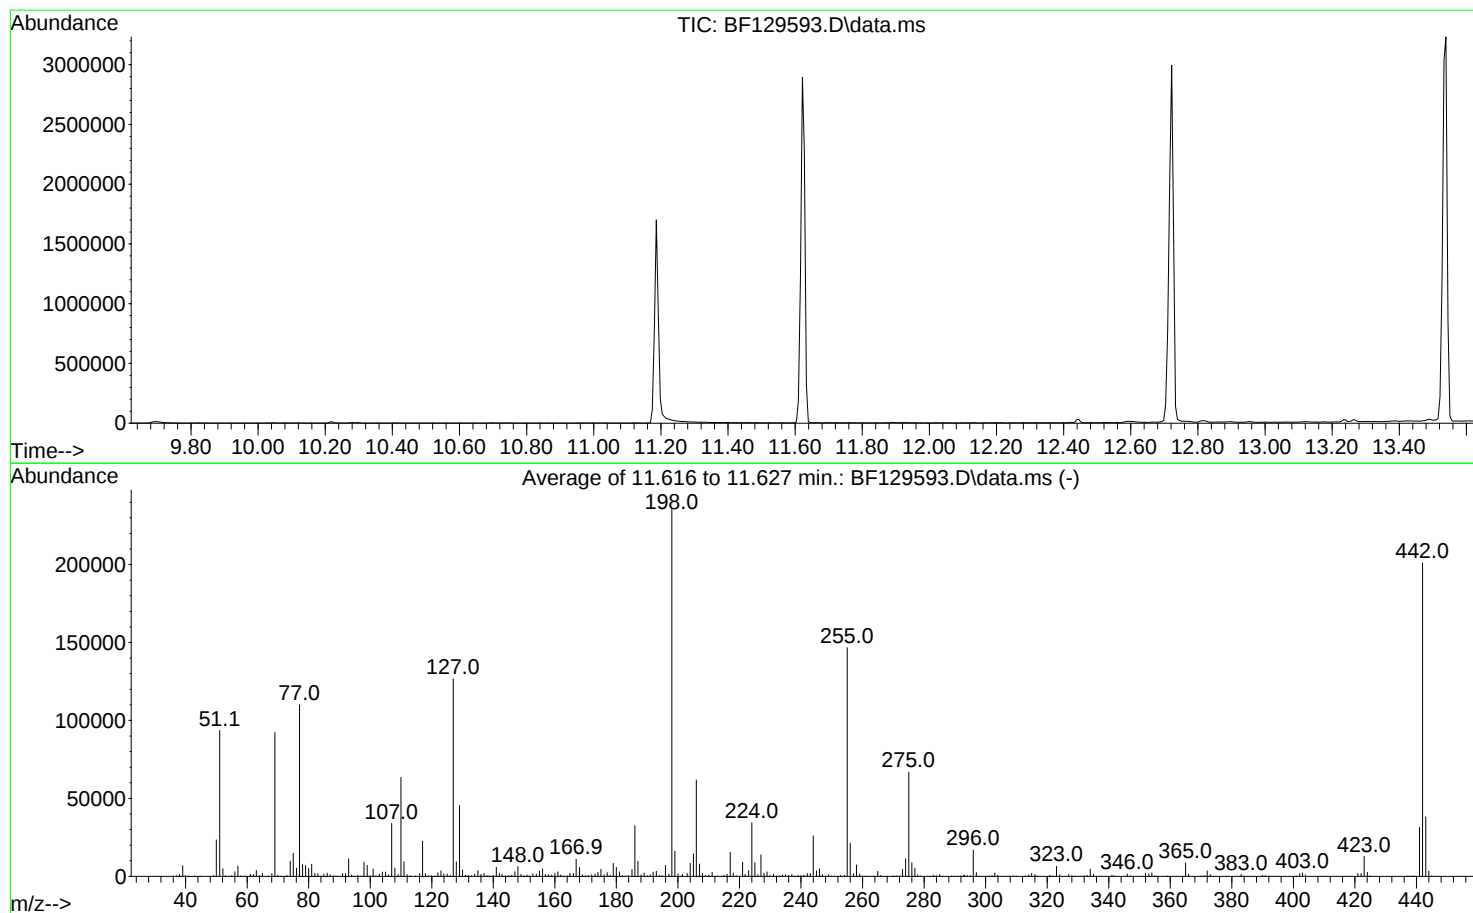




AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	93496	PASS
68	69	0.00	2	1.9	1776	PASS
69	198	0.00	100	39.1	92285	PASS
70	69	0.00	2	0.7	630	PASS
127	198	10	80	53.7	126688	PASS
197	198	0.00	2	0.6	1371	PASS
198	198	100	100	100.0	236032	PASS
199	198	5	9	6.8	16040	PASS
275	198	10	60	28.4	66941	PASS
365	198	1	100	3.7	8619	PASS
441	198	0.01	100	13.3	31407	PASS
442	442	50	100	100.0	201056	PASS
443	442	15	24	19.0	38194	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
Data File : BF129593.D
Acq On : 05 Aug 2022 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 08 04:54:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 16:27:34 2022
Response via : Initial Calibration

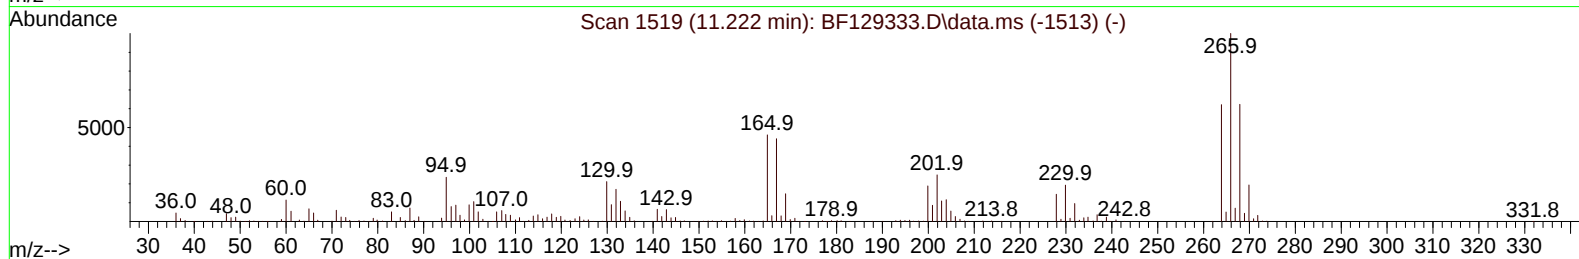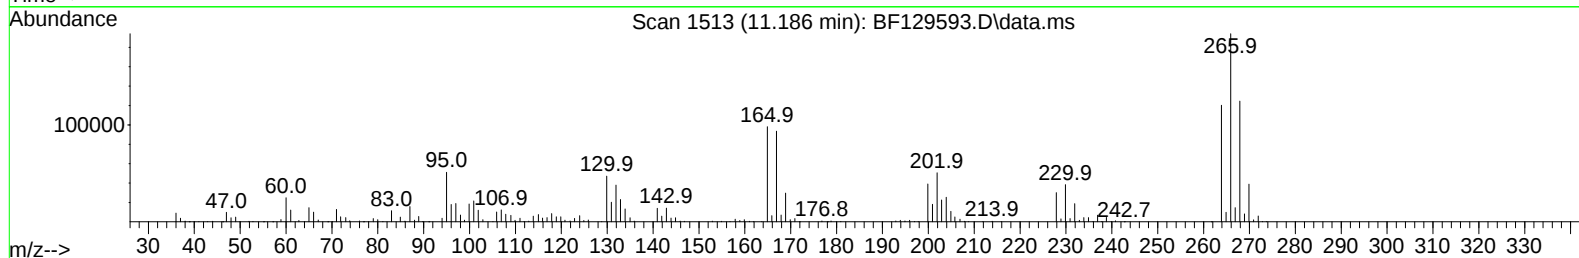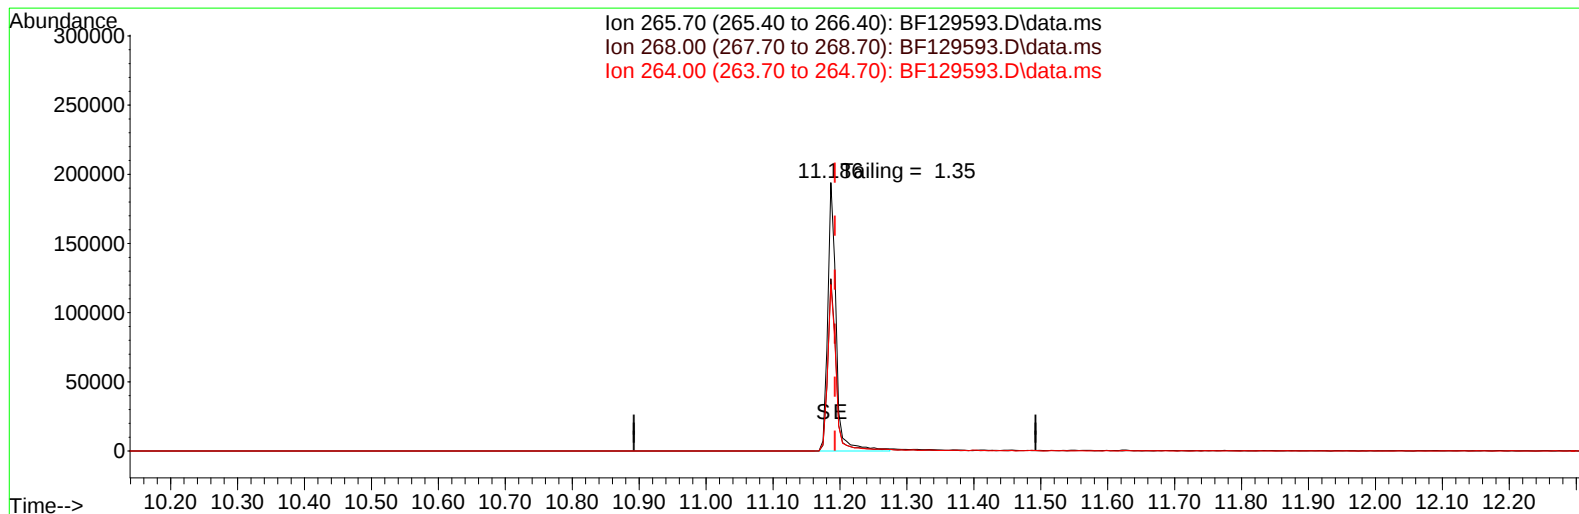

TIC: BF129593.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 29212.03 ng




response 172972

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.17
264.00	61.80	62.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
Data File : BF129593.D
Acq On : 05 Aug 2022 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 08 04:54:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 16:27:34 2022
Response via : Initial Calibration

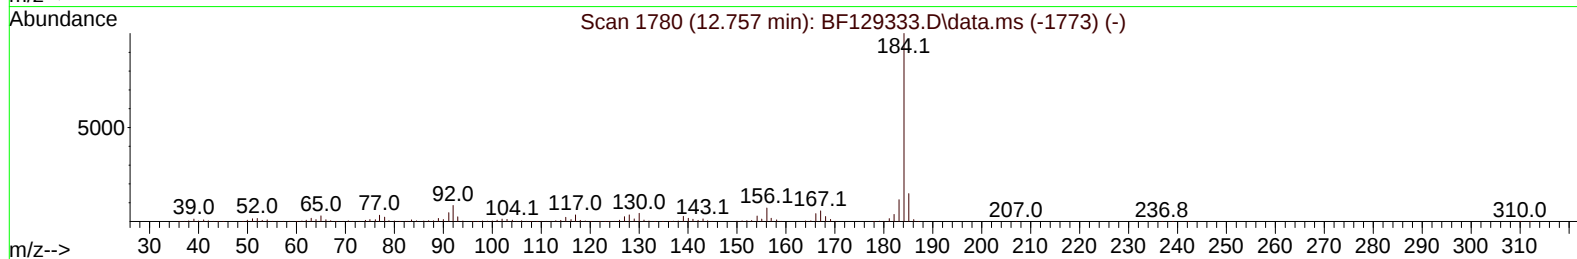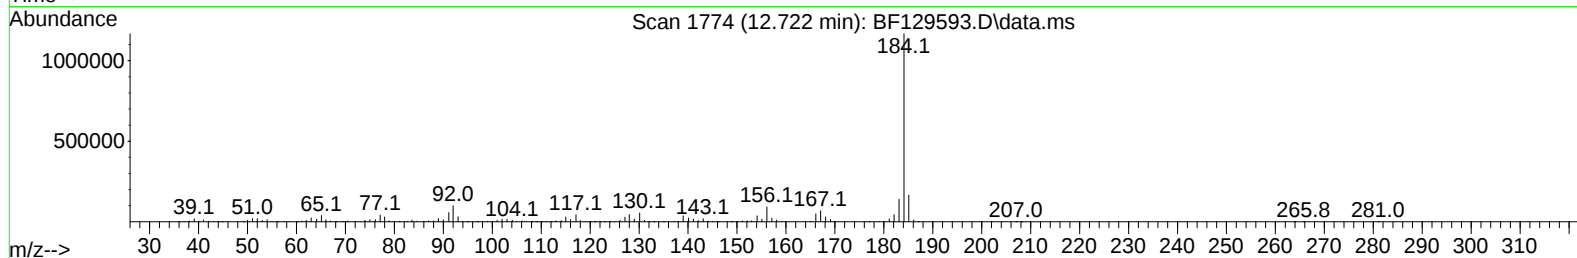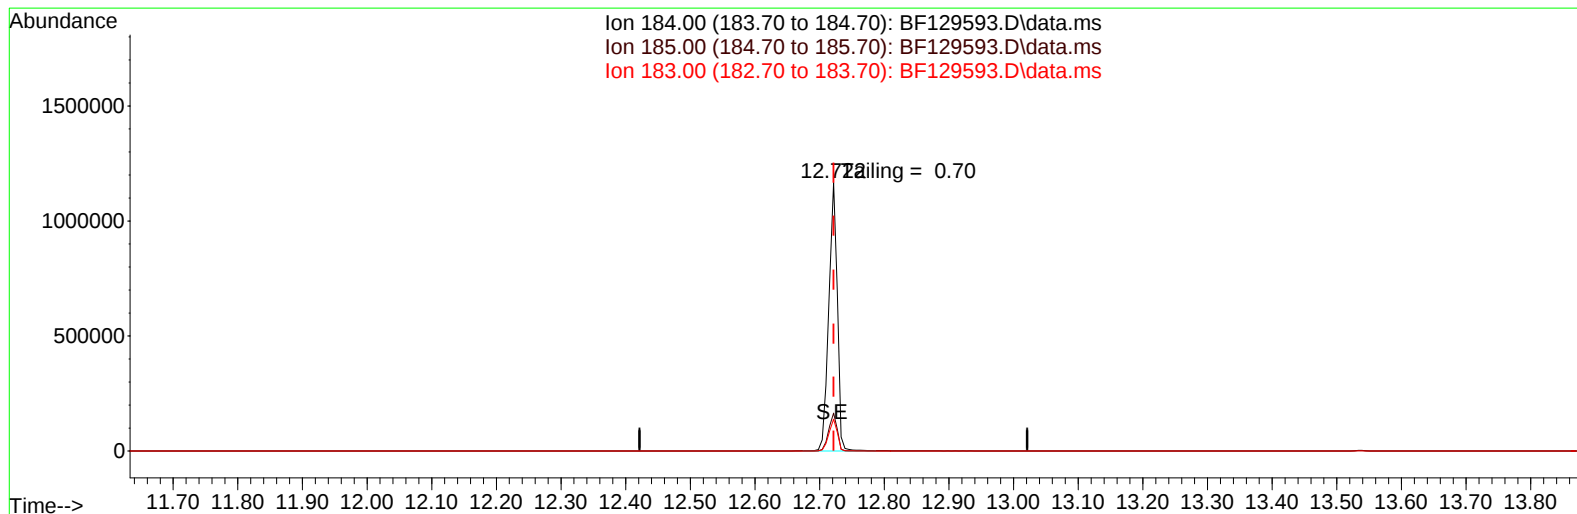

TIC: BF129593.D\data.ms

(77) Benzidine

12.722min (-0.000) 0.00 ng

response 1083570

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.17
183.00	11.60	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/5/2022	BNA_F	<u>BF129593.D</u>
Compound Name	Response	Retention Time
DDT	573788	13.539
DDD	6771	13.239
DDE	582	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7353	581141	1.27

Instrument :
BNA_F
ClientSampleId :
DFTPP