
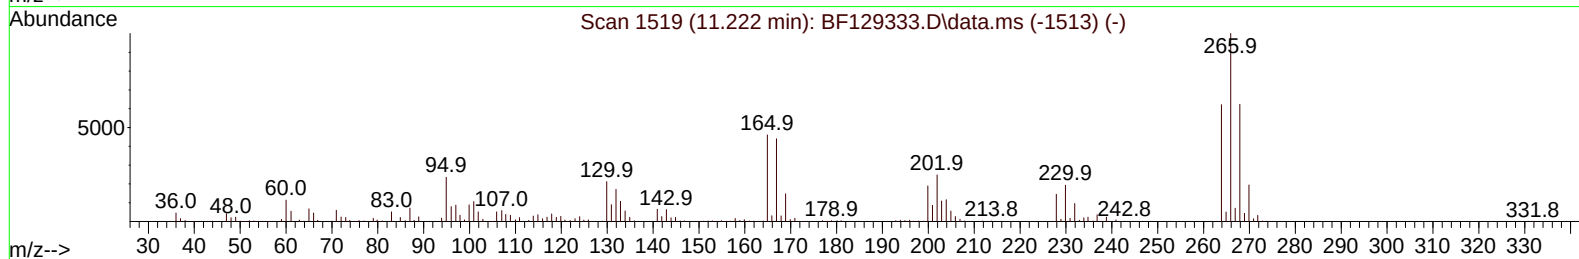
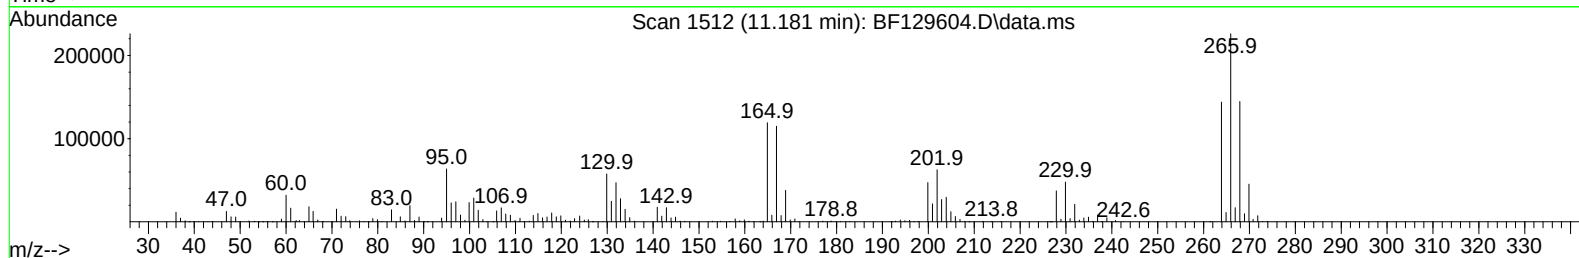


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
 Data File : BF129604.D
 Acq On : 05 Aug 2022 17:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 08 04:56:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 05 16:27:34 2022
 Response via : Initial Calibration

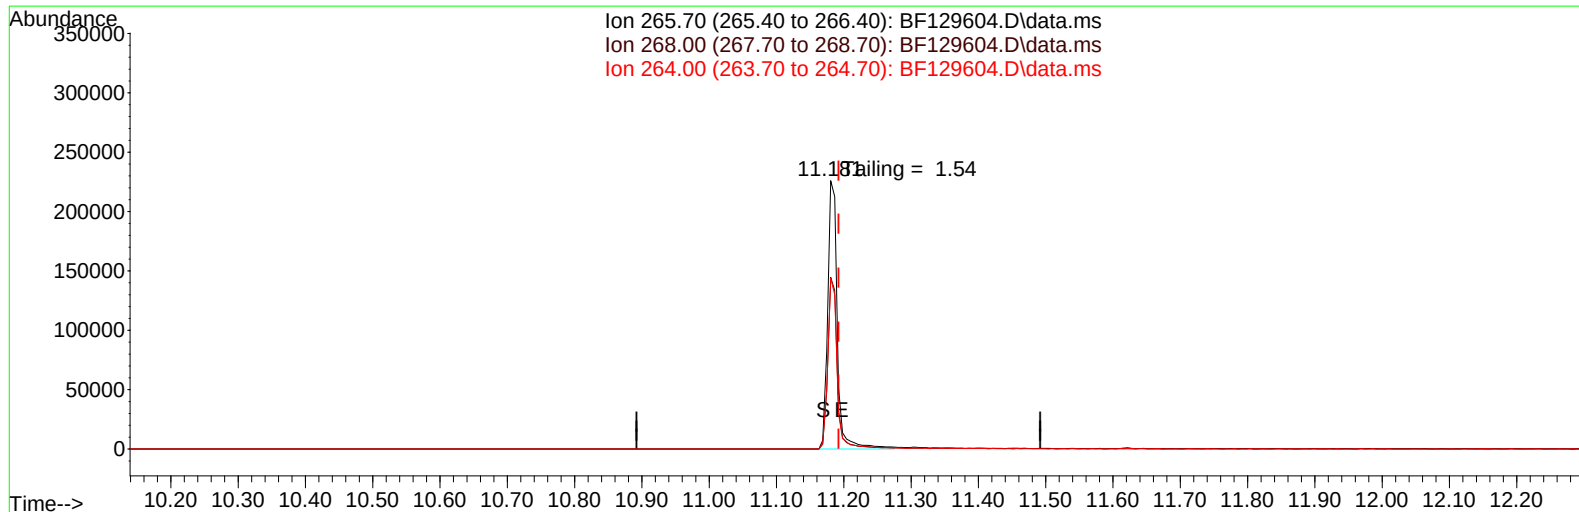

TIC: BF129604.D\data.ms

(70) Pentachlorophenol (C)

11.181min (-0.012) 220925.24 ng




response 226576

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.99
264.00	61.80	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
 Data File : BF129604.D
 Acq On : 05 Aug 2022 17:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 08 04:56:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 05 16:27:34 2022
 Response via : Initial Calibration

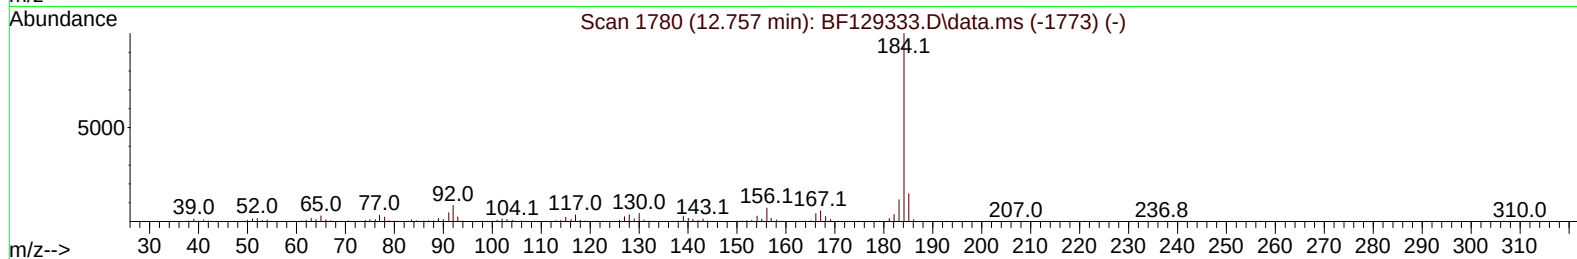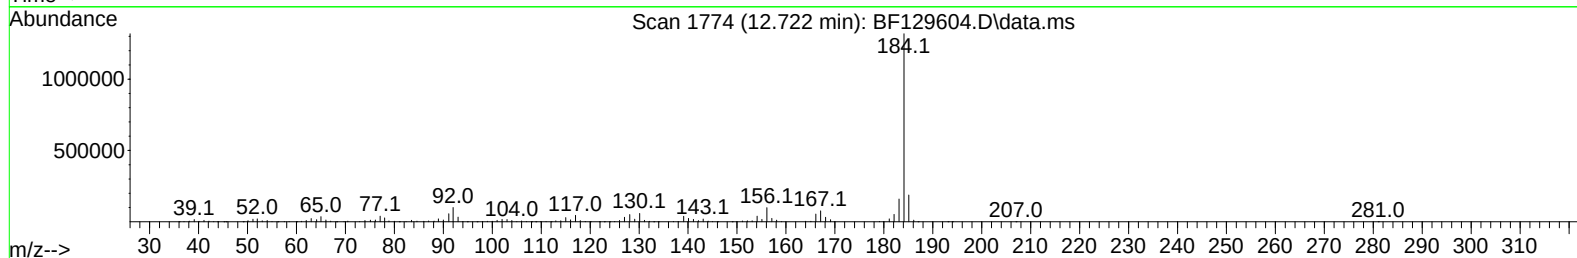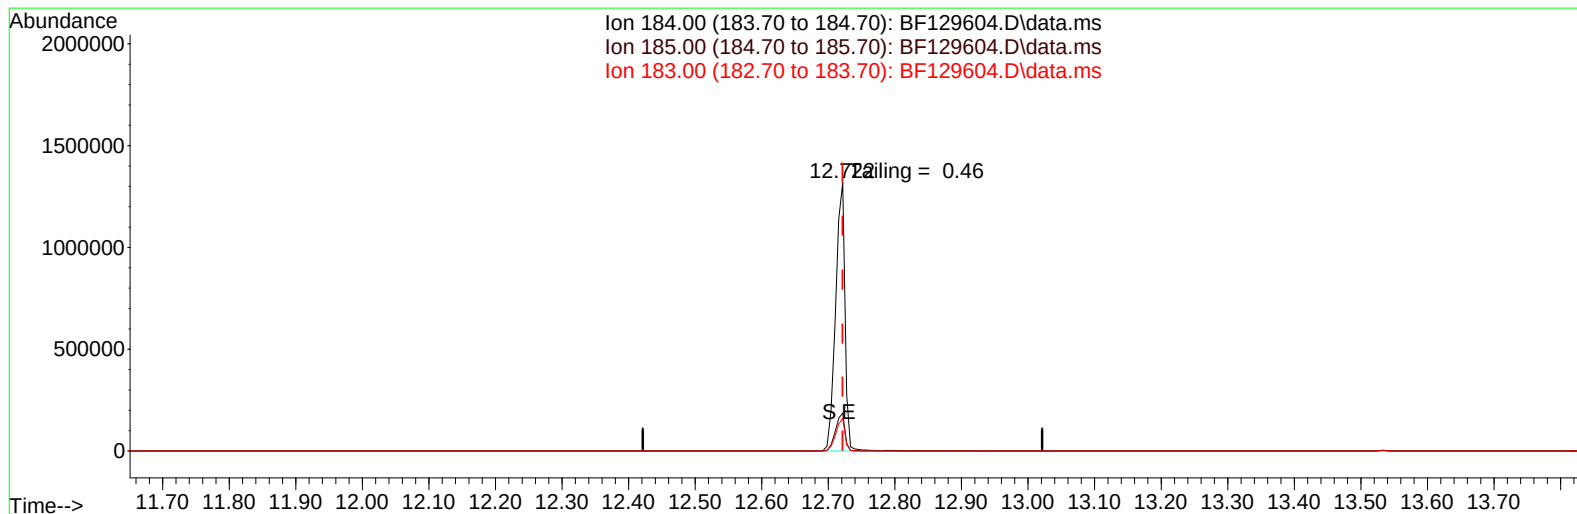

TIC: BF129604.D\data.ms

(77) Benzidine

12.722min (+ 0.000) 25870.47 ng

response 1282257


Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.23
183.00	11.60	12.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080522\
 Data File : BF129604.D
 Acq On : 05 Aug 2022 17:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 05 16:27:34 2022

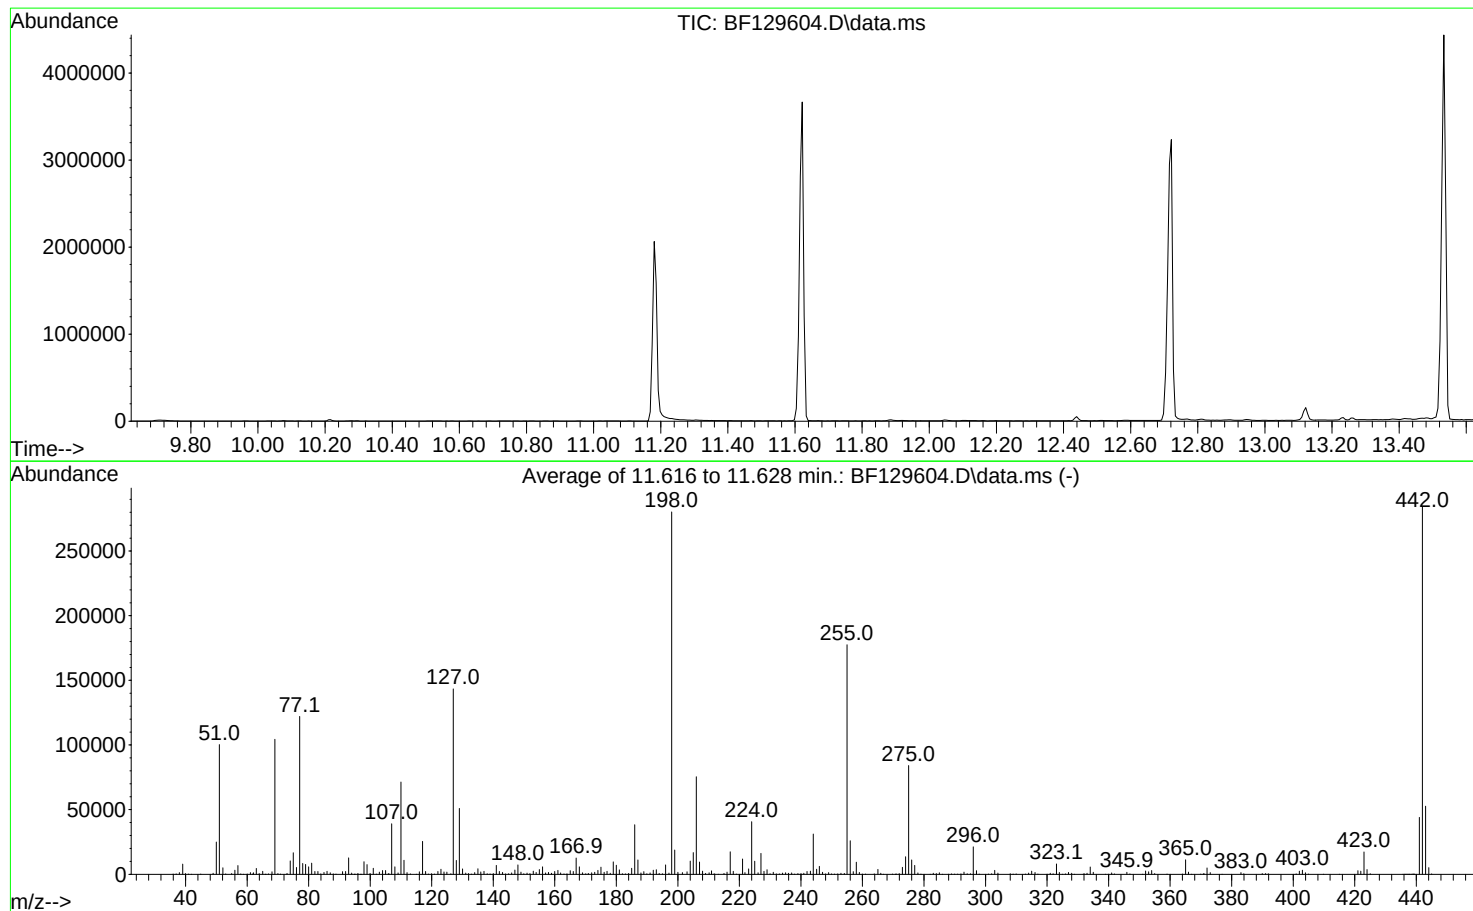

AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	100312	PASS
68	69	0.00	2	1.9	1977	PASS
69	198	0.00	100	37.3	104440	PASS
70	69	0.00	2	0.5	574	PASS
127	198	10	80	51.1	143333	PASS
197	198	0.00	2	0.3	924	PASS
198	198	100	100	100.0	280275	PASS
199	198	5	9	6.7	18727	PASS
275	198	10	60	30.0	84101	PASS
365	198	1	100	4.0	11259	PASS
441	198	0.01	100	15.7	43947	PASS
442	442	50	100	100.0	284523	PASS
443	442	15	24	18.5	52712	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/5/2022	BNA_F	<u>BF129604.D</u>
Compound Name	Response	Retention Time
DDT	718041	13.533
DDD	9794	13.233
DDE	1266	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11060	729101	1.52

Instrument :
BNA_F
ClientSampleId :
DFTPP