

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
 Data File : BF138799.D
 Acq On : 05 Aug 2024 22:36
 Operator : RC/JU
 Sample : P3387-02RE
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-9-Full Waste ClassRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138799.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	500	504	515	rVB	34035	50916	7.22%	0.744%
2	5.469	569	574	595	rVB	509004	688540	97.67%	10.055%
3	6.487	741	747	765	rBV	532473	704982	100.00%	10.295%
4	6.845	803	808	813	rVB	182965	224763	31.88%	3.282%
5	7.410	898	904	914	rBV	339240	439303	62.31%	6.415%
6	7.663	943	947	951	rBV	8409	10827	1.54%	0.158%
7	8.128	1019	1026	1042	rBV	197453	253876	36.01%	3.707%
8	8.445	1075	1080	1091	rBV	10436	21428	3.04%	0.313%
9	9.198	1203	1208	1217	rBV	553667	678580	96.25%	9.909%
10	9.739	1296	1300	1306	rVB	7723	9730	1.38%	0.142%
11	9.875	1318	1323	1328	rBV	169938	220564	31.29%	3.221%
12	9.969	1334	1339	1345	rBV2	11781	18389	2.61%	0.269%
13	10.669	1453	1458	1468	rBV	251159	323974	45.95%	4.731%
14	10.775	1472	1476	1486	rVB4	3019	7998	1.13%	0.117%
15	11.316	1563	1568	1571	rBV4	4979	7907	1.12%	0.115%
16	11.363	1571	1576	1579	rBV	164892	232730	33.01%	3.399%
17	11.439	1586	1589	1593	rVB	12272	13997	1.99%	0.204%
18	11.604	1611	1617	1621	rBV2	5657	8955	1.27%	0.131%
19	11.869	1657	1662	1663	rBV	14240	16925	2.40%	0.247%
20	11.892	1663	1666	1672	rVB3	41040	55016	7.80%	0.803%
21	11.980	1677	1681	1690	rVB	25793	46252	6.56%	0.675%
22	12.057	1690	1694	1700	rBV9	4073	9501	1.35%	0.139%
23	12.163	1708	1712	1714	rBV	9837	10919	1.55%	0.159%
24	12.192	1714	1717	1722	rVB	15209	19117	2.71%	0.279%
25	12.416	1751	1755	1758	rBV	10550	15464	2.19%	0.226%
26	12.451	1758	1761	1764	rVV4	7624	10792	1.53%	0.158%
27	12.510	1767	1771	1774	rVB2	10371	13871	1.97%	0.203%
28	12.580	1778	1783	1788	rBV	213582	274110	38.88%	4.003%
29	12.674	1796	1799	1803	rBV	19184	25155	3.57%	0.367%
30	12.810	1812	1822	1827	rBV	176228	259212	36.77%	3.785%
31	12.857	1827	1830	1835	rVB2	9688	14404	2.04%	0.210%
32	12.951	1835	1846	1853	rBV	495135	662969	94.04%	9.681%
33	13.027	1853	1859	1864	rBV2	17206	35312	5.01%	0.516%
34	13.133	1870	1877	1881	rBV	26484	50834	7.21%	0.742%
35	13.204	1885	1889	1892	rVV	17440	24475	3.47%	0.357%
36	13.239	1892	1895	1901	rVB2	15972	24463	3.47%	0.357%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
 Data File : BF138799.D
 Acq On : 05 Aug 2024 22:36
 Operator : RC/JU
 Sample : P3387-02RE
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-9-Full Waste ClassRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	13.333	1908	1911	1913	rBV	7729	7922	1.12%	0.116%
38	13.369	1914	1917	1921	rVV3	8939	14868	2.11%	0.217%
39	13.427	1922	1927	1936	rVV	54582	114476	16.24%	1.672%
40	13.504	1936	1940	1944	rVB2	14697	20560	2.92%	0.300%
41	13.645	1961	1964	1972	rVB	15712	25879	3.67%	0.378%
42	13.757	1978	1983	1985	rBV	20588	31207	4.43%	0.456%
43	13.780	1985	1987	1990	rVV	7973	9958	1.41%	0.145%
44	13.863	1997	2001	2009	rVB4	20545	45462	6.45%	0.664%
45	14.004	2019	2025	2029	rBV2	177022	320821	45.51%	4.685%
46	14.110	2040	2043	2048	rVB2	17529	22506	3.19%	0.329%
47	14.751	2148	2152	2163	rVB2	76926	113604	16.11%	1.659%
48	14.915	2177	2180	2183	rVB	20752	25258	3.58%	0.369%
49	15.051	2197	2203	2209	rBV	79167	184152	26.12%	2.689%
50	15.351	2250	2254	2260	rVB	42146	64056	9.09%	0.935%
51	15.415	2260	2265	2270	rBV	55411	88775	12.59%	1.296%
52	15.474	2270	2275	2286	rVB2	85487	157107	22.29%	2.294%
53	15.910	2345	2349	2355	rVB	26811	43774	6.21%	0.639%
54	16.951	2521	2526	2533	rBV2	20842	46832	6.64%	0.684%
55	17.398	2598	2602	2609	rVB2	12799	24525	3.48%	0.358%




Sum of corrected areas: 6847992

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
Data File : BF138799.D
Acq On : 05 Aug 2024 22:36
Operator : RC/JU
Sample : P3387-02RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-9-Full Waste ClassRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

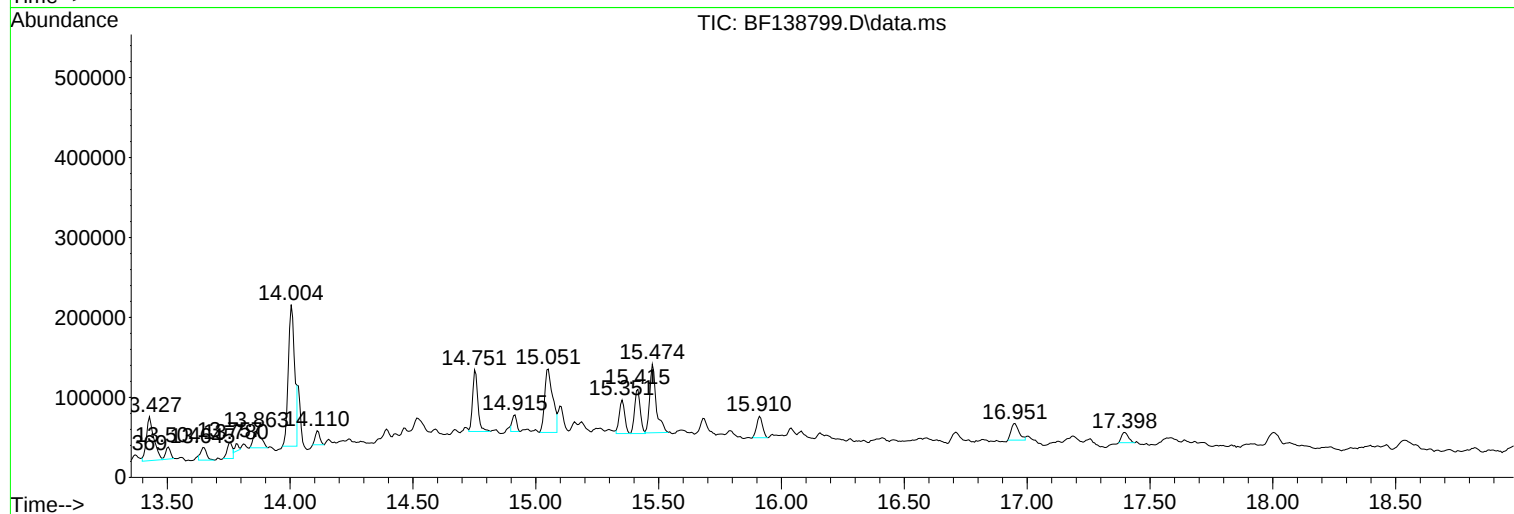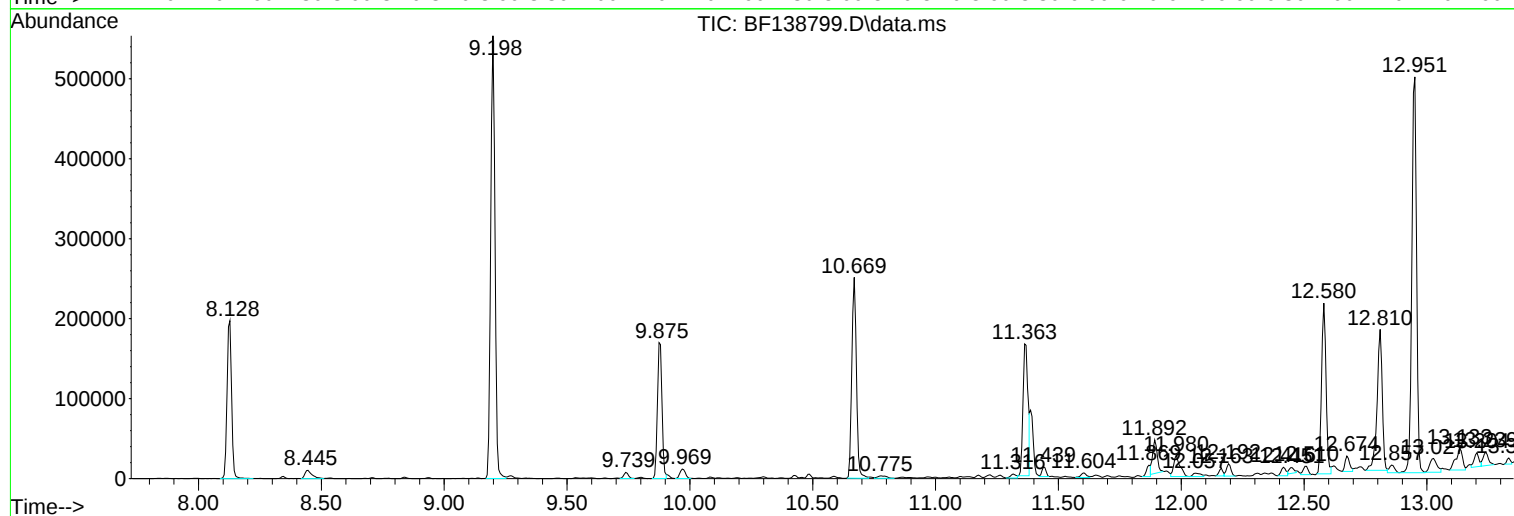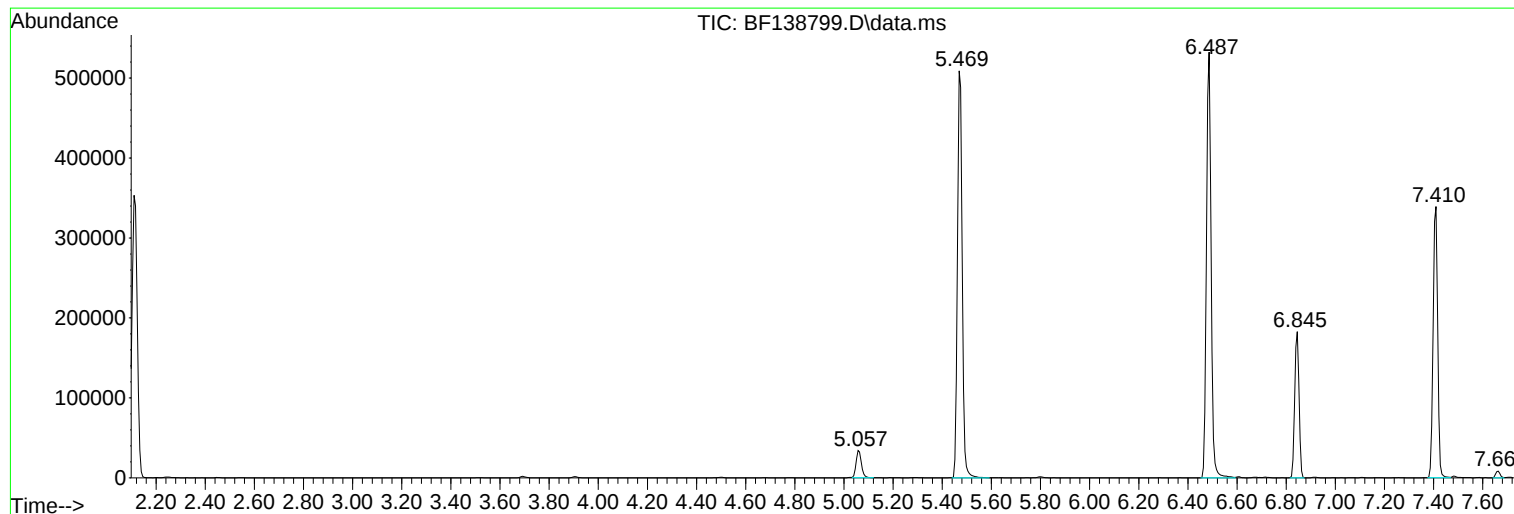

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
Data File : BF138799.D
Acq On : 05 Aug 2024 22:36
Operator : RC/JU
Sample : P3387-02RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-9-Full Waste ClassRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
Data File : BF138799.D
Acq On : 05 Aug 2024 22:36
Operator : RC/JU
Sample : P3387-02RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-9-Full Waste ClassRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------