

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
 Data File : BF138800.D
 Acq On : 05 Aug 2024 23:08
 Operator : RC/JU
 Sample : P3362-04RE
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-11978RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.151	3	10	17	rVB	708727	1135615	89.43%	8.692%
2	3.404	219	223	231	rBV	7272	18120	1.43%	0.139%
3	5.081	503	508	522	rVB	48904	83627	6.59%	0.640%
4	5.481	570	576	594	rBV	959655	1269829	100.00%	9.719%
5	6.486	741	747	767	rBV	864148	1235454	97.29%	9.456%
6	6.845	803	808	813	rVB	216582	260654	20.53%	1.995%
7	7.410	898	904	909	rBV	576994	759778	59.83%	5.815%
8	7.663	943	947	952	rBB	14240	17211	1.36%	0.132%
9	8.128	1020	1026	1041	rVB	233710	299789	23.61%	2.295%
10	8.439	1075	1079	1092	rBV	16247	31372	2.47%	0.240%
11	9.198	1202	1208	1213	rBV	929419	1163207	91.60%	8.903%
12	9.510	1257	1261	1264	rBV	46122	59061	4.65%	0.452%
13	9.880	1318	1324	1327	rBV	206225	264804	20.85%	2.027%
14	9.910	1327	1329	1334	rVB	28071	29932	2.36%	0.229%
15	9.969	1334	1339	1346	rBV2	19445	31505	2.48%	0.241%
16	10.080	1354	1358	1362	rBV2	14009	17217	1.36%	0.132%
17	10.427	1413	1417	1422	rVB	18458	22556	1.78%	0.173%
18	10.492	1422	1428	1434	rBV7	6022	15016	1.18%	0.115%
19	10.669	1453	1458	1468	rBV	436129	573604	45.17%	4.390%
20	10.774	1472	1476	1485	rVB2	54807	90403	7.12%	0.692%
21	10.974	1503	1510	1513	rBV3	9480	14883	1.17%	0.114%
22	11.127	1533	1536	1540	rVV3	8964	13854	1.09%	0.106%
23	11.174	1540	1544	1548	rVV2	19129	29277	2.31%	0.224%
24	11.216	1548	1551	1555	rVV2	12420	19792	1.56%	0.151%
25	11.263	1555	1559	1564	rVB	13399	18191	1.43%	0.139%
26	11.369	1571	1577	1579	rBV	199392	288274	22.70%	2.206%
27	11.386	1579	1580	1585	rVV	151912	155318	12.23%	1.189%
28	11.439	1585	1589	1593	rVV	36086	43400	3.42%	0.332%
29	11.598	1610	1616	1624	rBV3	20134	45238	3.56%	0.346%
30	11.768	1638	1645	1651	rVB10	7735	18793	1.48%	0.144%
31	11.868	1657	1662	1663	rBV	29172	37708	2.97%	0.289%
32	11.892	1663	1666	1671	rVV2	75332	111253	8.76%	0.852%
33	11.945	1671	1675	1677	rVV	17422	26090	2.05%	0.200%
34	11.980	1677	1681	1689	rVB	61035	103562	8.16%	0.793%
35	12.163	1708	1712	1715	rBV	23255	32233	2.54%	0.247%
36	12.192	1715	1717	1721	rVB2	25009	27600	2.17%	0.211%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
 Data File : BF138800.D
 Acq On : 05 Aug 2024 23:08
 Operator : RC/JU
 Sample : P3362-04RE
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-11978RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	12.310	1733	1737	1740	rBV3	11250	18528	1.46%	0.142%
38	12.416	1751	1755	1758	rBV	26107	40442	3.18%	0.310%
39	12.451	1758	1761	1767	rVV5	28667	52044	4.10%	0.398%
40	12.510	1767	1771	1776	rVB	47512	66025	5.20%	0.505%
41	12.580	1778	1783	1788	rBV	466902	604383	47.60%	4.626%
42	12.645	1788	1794	1796	rVV2	11385	18906	1.49%	0.145%
43	12.674	1796	1799	1802	rVB2	15692	16575	1.31%	0.127%
44	12.727	1804	1808	1812	rBV3	16804	22716	1.79%	0.174%
45	12.810	1815	1822	1828	rBV	397447	597990	47.09%	4.577%
46	12.857	1828	1830	1836	rVB2	20418	27362	2.15%	0.209%
47	12.951	1838	1846	1854	rBV	810755	1099120	86.56%	8.413%
48	13.027	1854	1859	1867	rBV3	36718	77238	6.08%	0.591%
49	13.133	1870	1877	1881	rVB3	52370	111781	8.80%	0.856%
50	13.204	1886	1889	1892	rBV2	29746	37218	2.93%	0.285%
51	13.239	1892	1895	1899	rBV2	33453	41763	3.29%	0.320%
52	13.333	1908	1911	1914	rBV2	23705	31844	2.51%	0.244%
53	13.380	1914	1919	1923	rVV2	95310	144570	11.38%	1.107%
54	13.645	1962	1964	1969	rVB	30493	39820	3.14%	0.305%
55	13.757	1979	1983	1986	rBV	42985	66596	5.24%	0.510%
56	13.810	1990	1992	1997	rVV2	17167	22486	1.77%	0.172%
57	13.862	1998	2001	2003	rBV2	20381	25497	2.01%	0.195%
58	14.004	2017	2025	2038	rBV3	236681	638205	50.26%	4.885%
59	14.627	2128	2131	2136	rBV	29397	41934	3.30%	0.321%
60	15.051	2198	2203	2210	rBV	131319	270463	21.30%	2.070%
61	15.162	2218	2222	2232	rVB3	26287	68720	5.41%	0.526%
62	15.351	2250	2254	2260	rVB	59272	92814	7.31%	0.710%
63	15.415	2260	2265	2270	rVV	71746	111020	8.74%	0.850%
64	15.474	2270	2275	2289	rVB2	96951	192321	15.15%	1.472%
65	15.909	2345	2349	2354	rVB2	26418	41380	3.26%	0.317%
66	16.703	2481	2484	2491	rBV6	12577	18408	1.45%	0.141%
67	16.951	2520	2526	2530	rBV2	27380	62728	4.94%	0.480%




Sum of corrected areas: 13065117

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
Data File : BF138800.D
Acq On : 05 Aug 2024 23:08
Operator : RC/JU
Sample : P3362-04RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11978RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

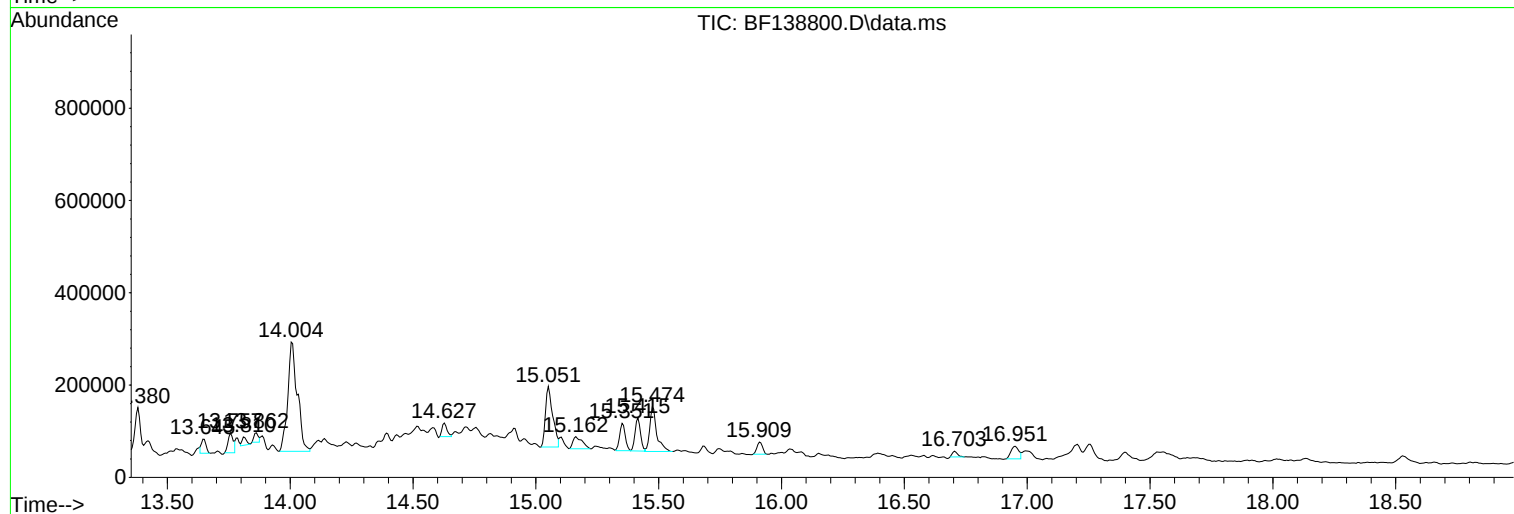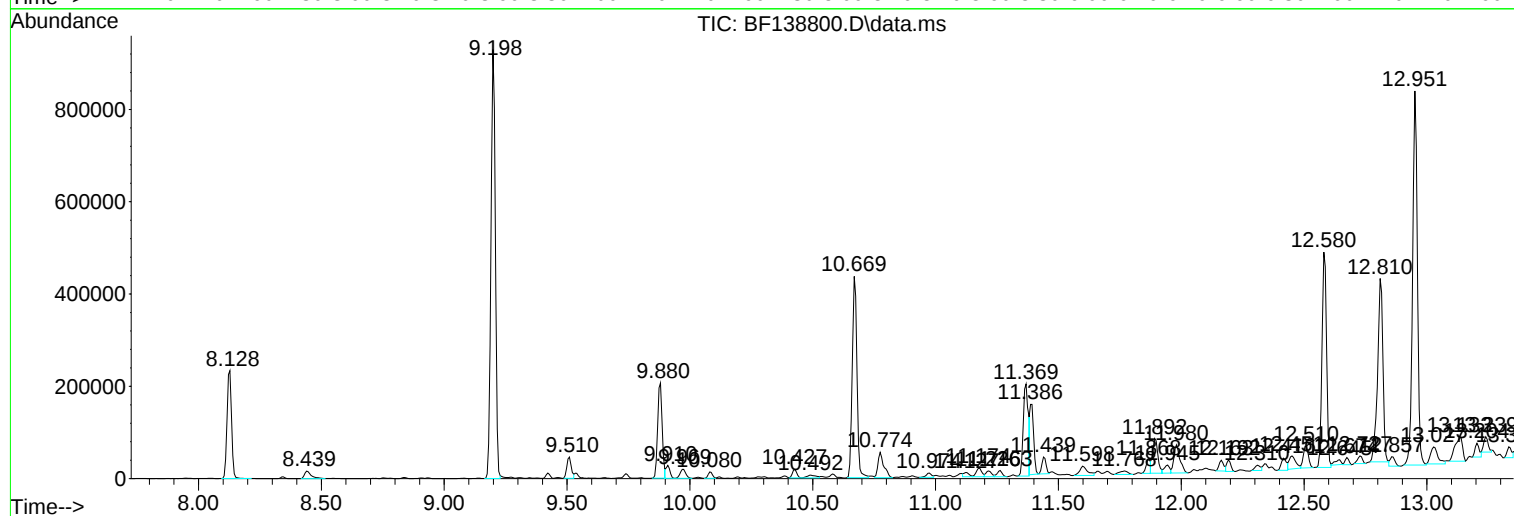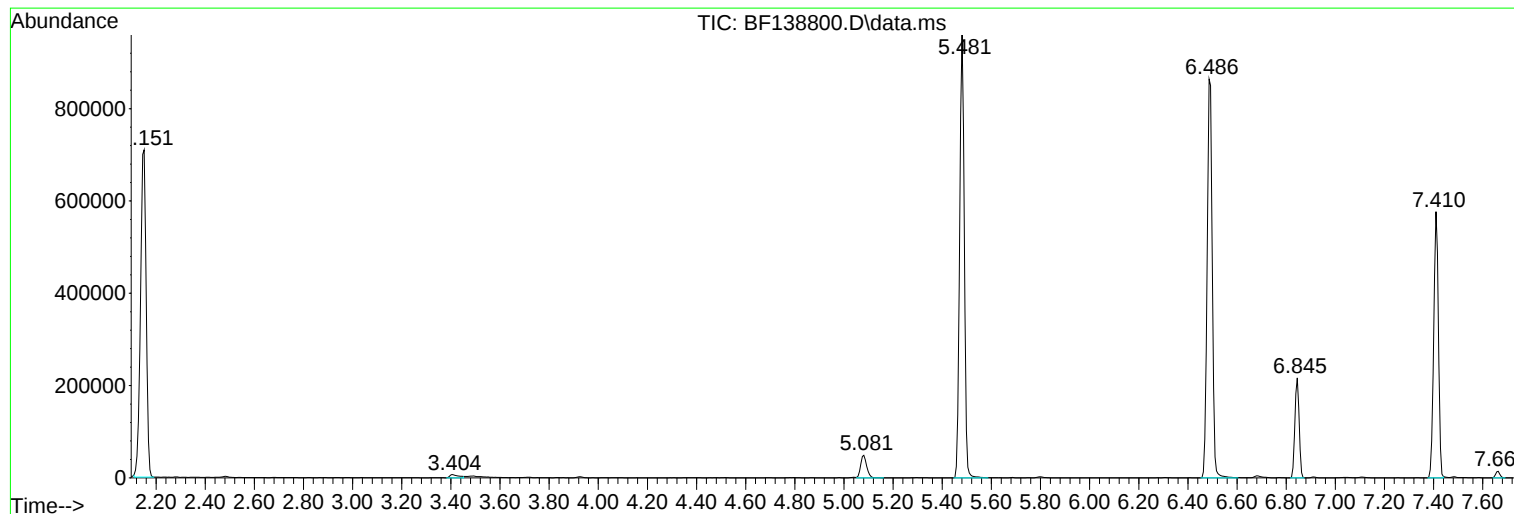

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
Data File : BF138800.D
Acq On : 05 Aug 2024 23:08
Operator : RC/JU
Sample : P3362-04RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11978RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
Data File : BF138800.D
Acq On : 05 Aug 2024 23:08
Operator : RC/JU
Sample : P3362-04RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11978RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------