
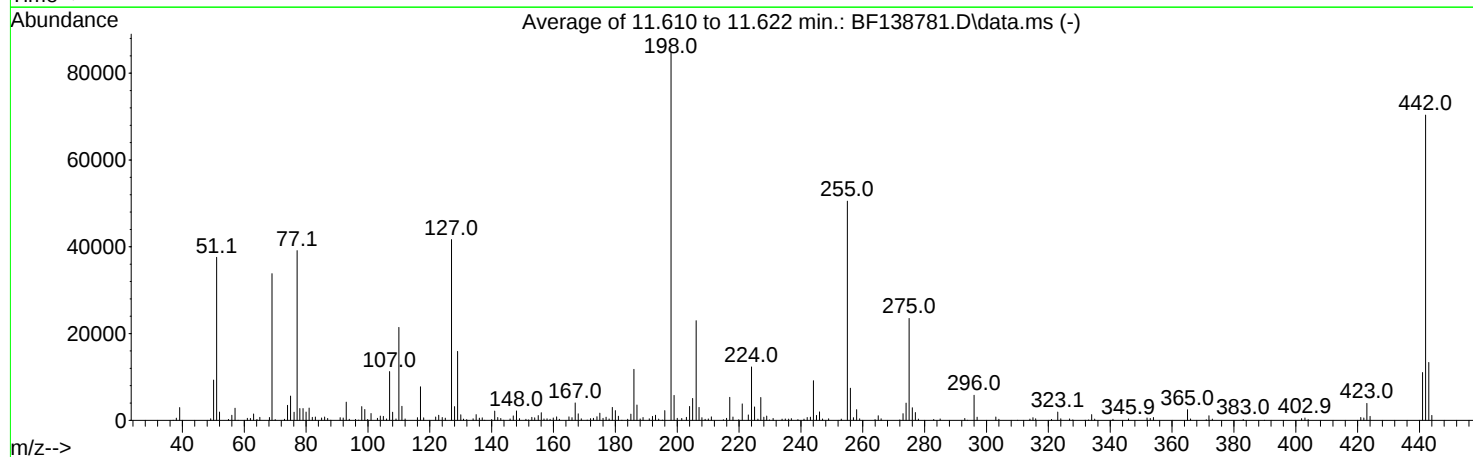


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
Data File : BF138781.D
Acq On : 05 Aug 2024 12:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

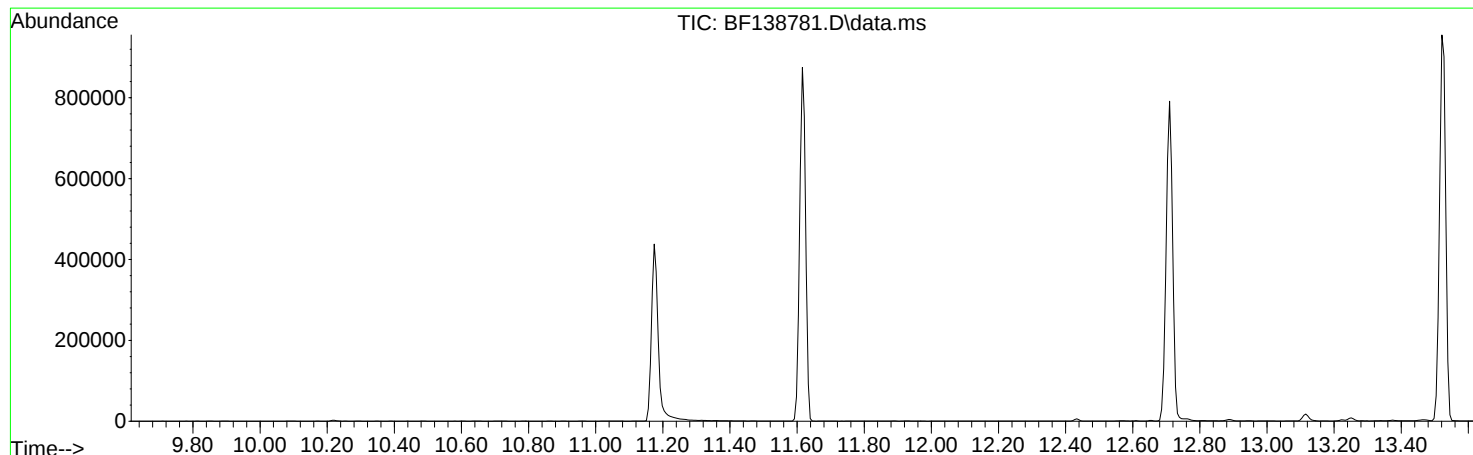




AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	37563	PASS
68	69	0.00	2	2.0	670	PASS
69	198	0.00	100	39.9	33795	PASS
70	69	0.00	2	0.6	188	PASS
127	198	10	80	49.1	41661	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84763	PASS
199	198	5	9	6.8	5769	PASS
275	198	10	60	27.7	23496	PASS
365	198	1	100	2.9	2490	PASS
441	198	0.01	100	13.0	11024	PASS
442	442	50	100	100.0	70355	PASS
443	442	15	24	19.0	13339	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
Data File : BF138781.D
Acq On : 05 Aug 2024 12:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 05 14:08:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

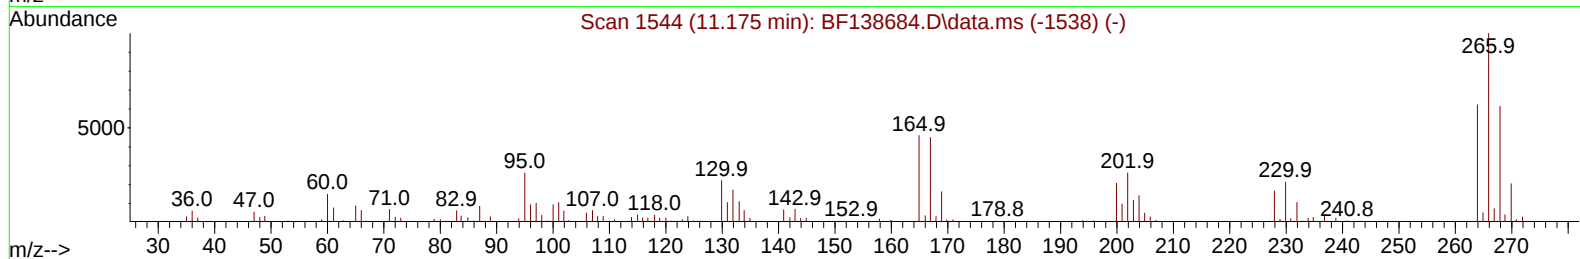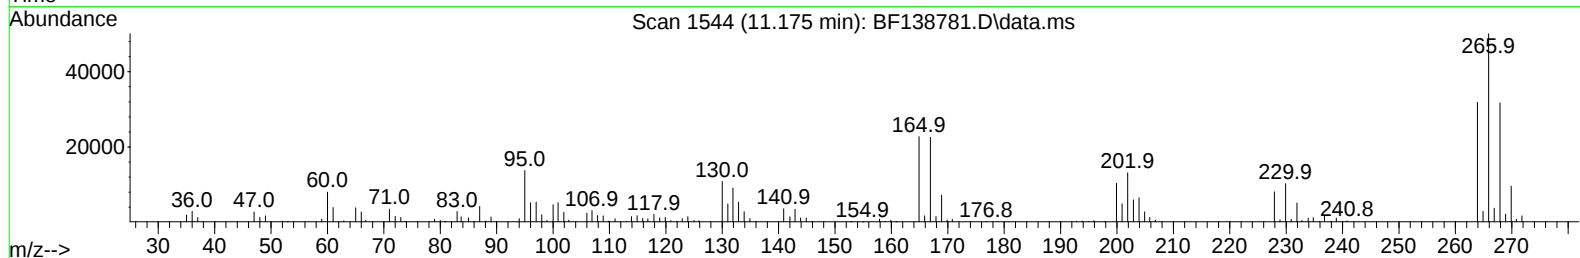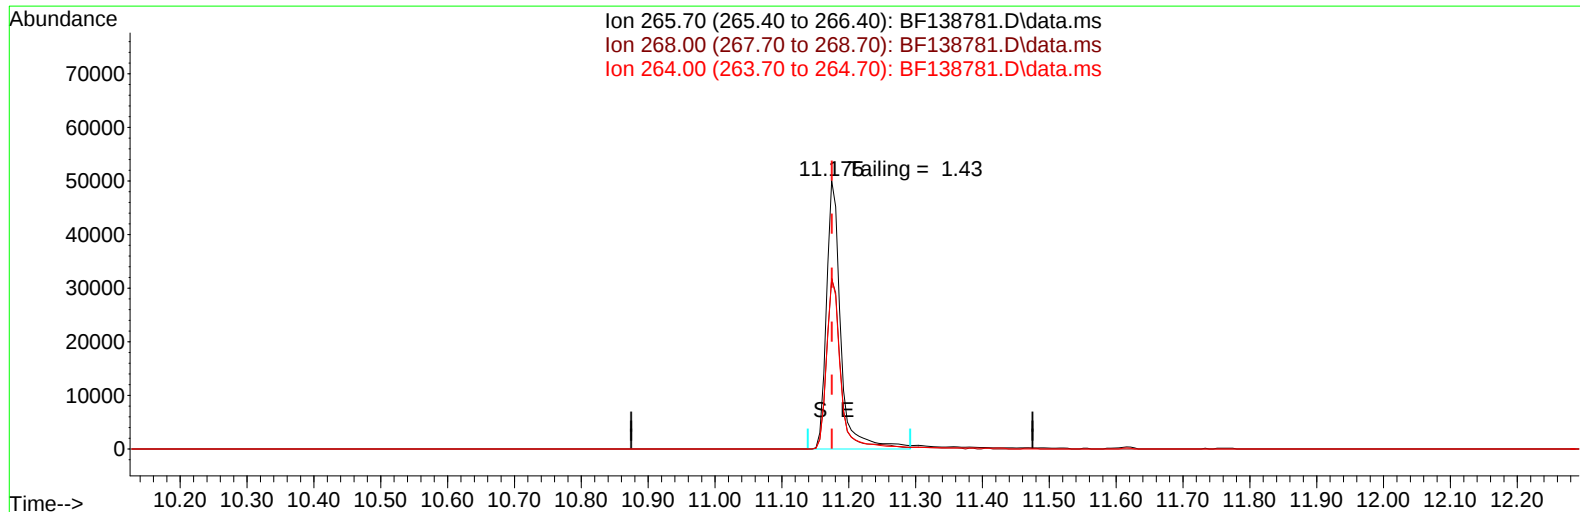

TIC: BF138781.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.001) 36576.28 ng




response 75010

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.39
264.00	62.20	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080524\
Data File : BF138781.D
Acq On : 05 Aug 2024 12:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 05 14:08:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

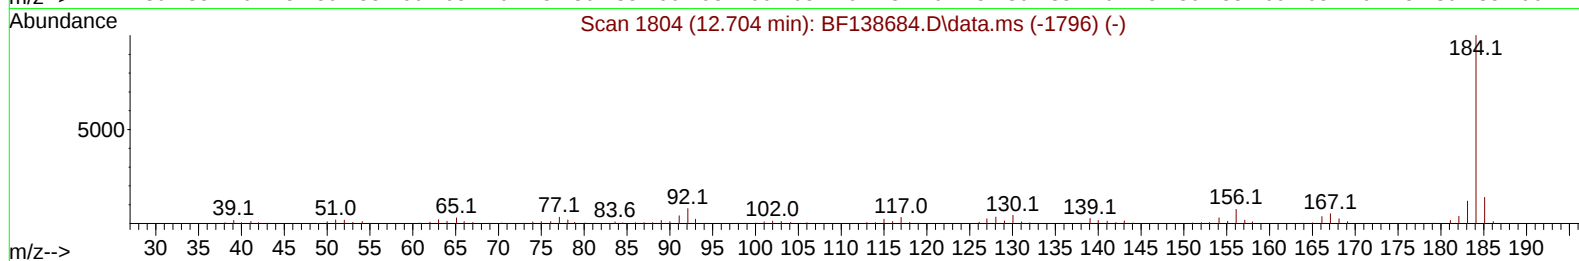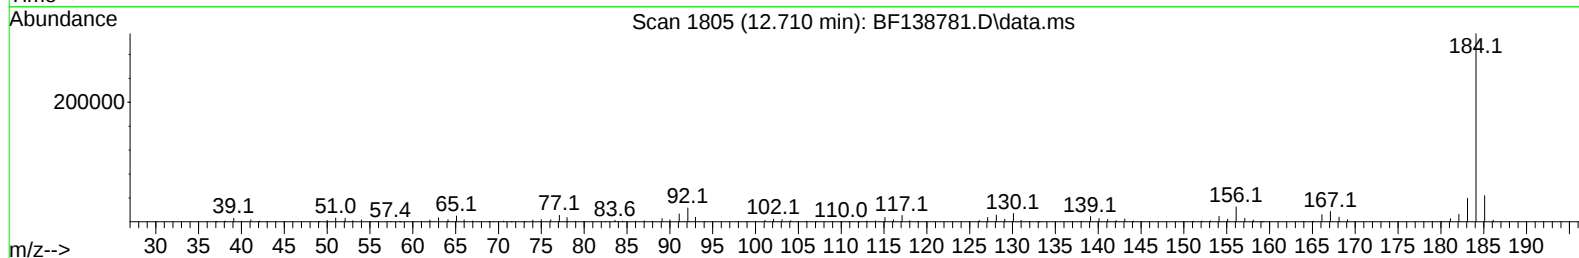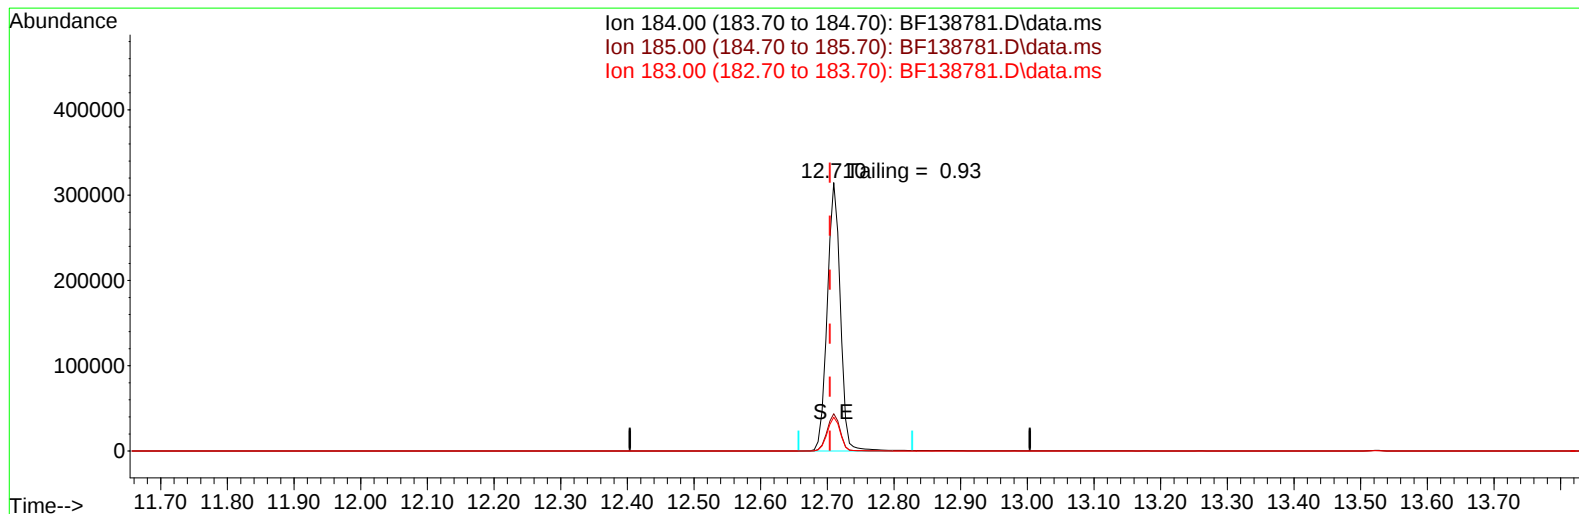

TIC: BF138781.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 427893

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.90
183.00	12.00	12.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/5/2024	BNA_F	<u>BF138781.D</u>
Compound Name	Response	Retention Time
DDT	240263	13.521
DDD	3969	13.251
DDE	1424	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5393	245656	2.20

Instrument :
BNA_F
ClientSampleId :
DFTPP