
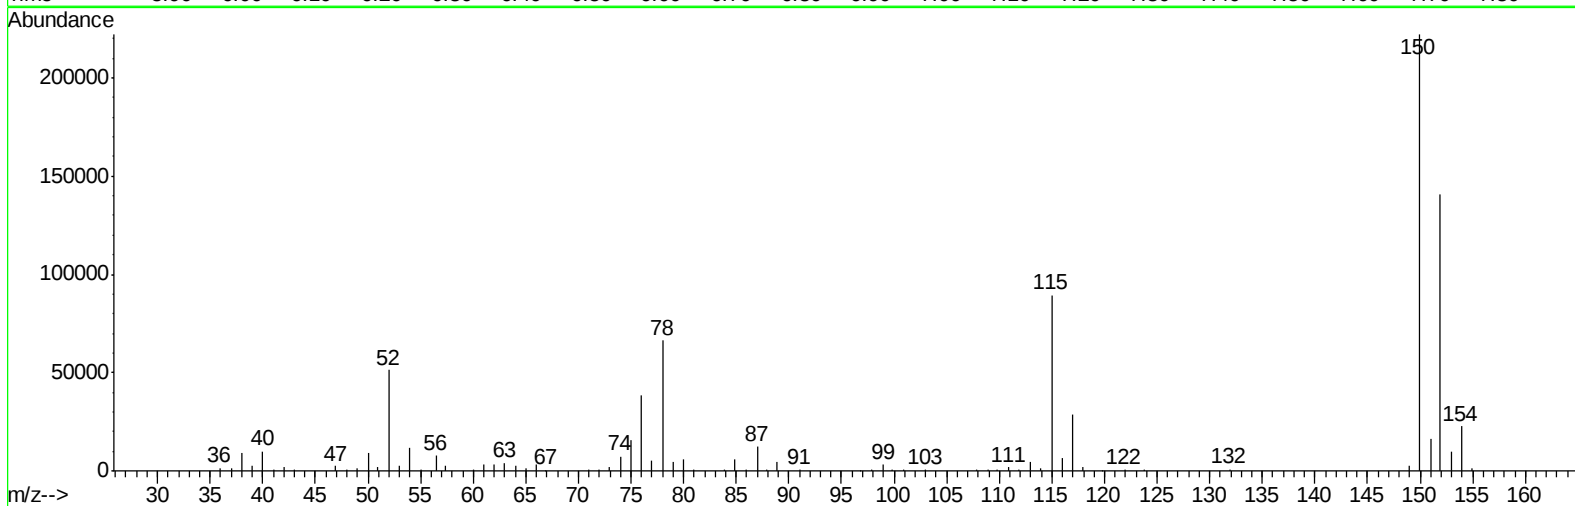


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080619\
Data File : BF116012.D
Acq On : 6 Aug 2019 14:49
Operator : HP/JU
Sample : K4135-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Aug 07 01:13:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:31:51 2019
Response via : Initial Calibration

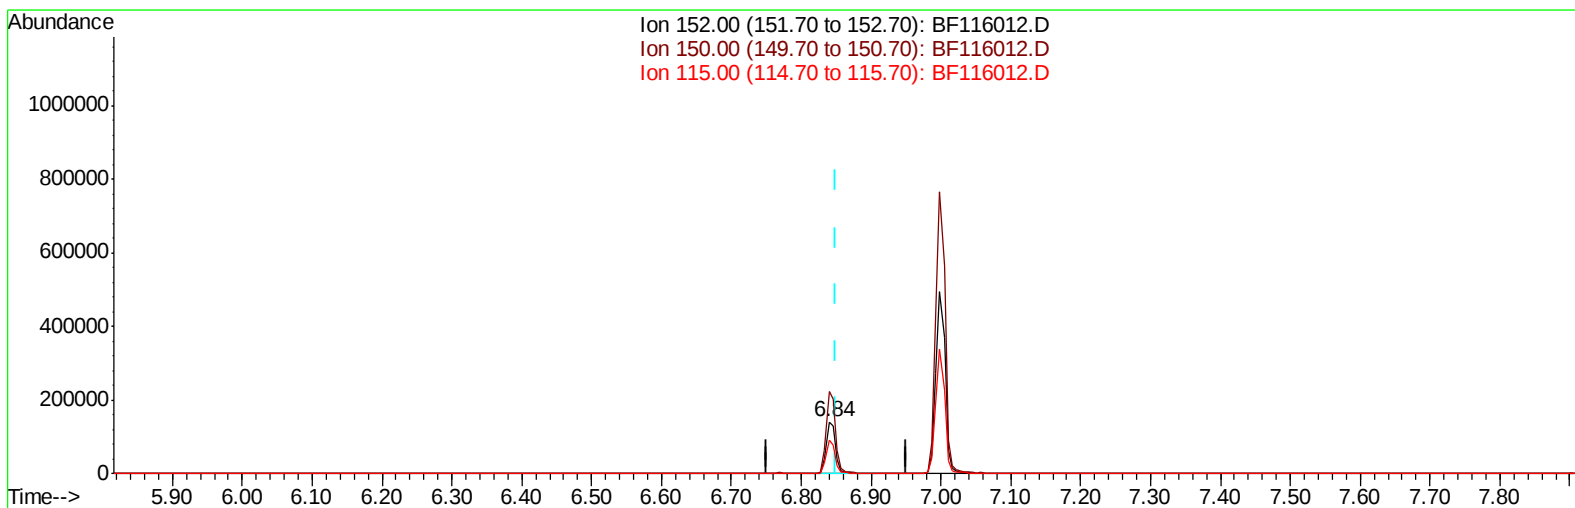

TIC: BF116012.D

(1) 1,4-Dichlorobenzene-d4 (I)

6.840min (-0.012) 20.00ng

response 130240

Ion	Exp%	Act%
152.00	100	100
150.00	159.20	157.99
115.00	64.80	63.64
0.00	0.00	0.00