


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080619\
 Data File : BF116000.D
 Acq On : 6 Aug 2019 8:51
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

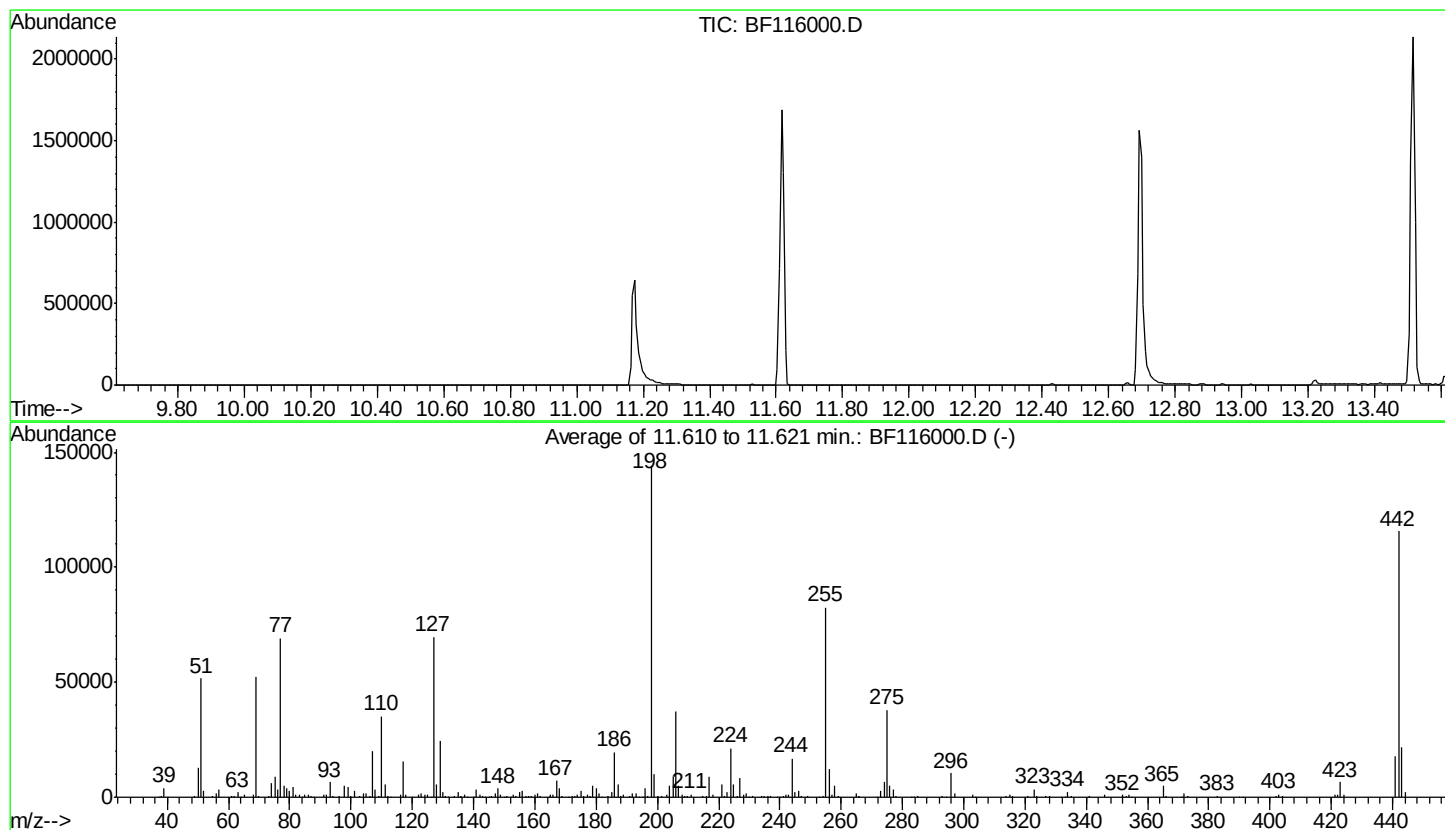

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	51624	PASS
68	69	0.00	2	1.8	928	PASS
69	198	0.00	100	36.3	52408	PASS
70	69	0.00	2	0.6	334	PASS
127	198	10	80	48.4	69762	PASS
197	198	0.00	2	0.6	851	PASS
198	198	100	100	100.0	144181	PASS
199	198	5	9	6.9	9978	PASS
275	198	10	60	26.3	37898	PASS
365	198	1	100	3.3	4779	PASS
441	198	0.01	100	12.5	18002	PASS
442	198	50	100	80.2	115578	PASS
443	442	15	24	18.9	21833	PASS