


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080619\
 Data File : BF116015.D
 Acq On : 6 Aug 2019 16:10
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

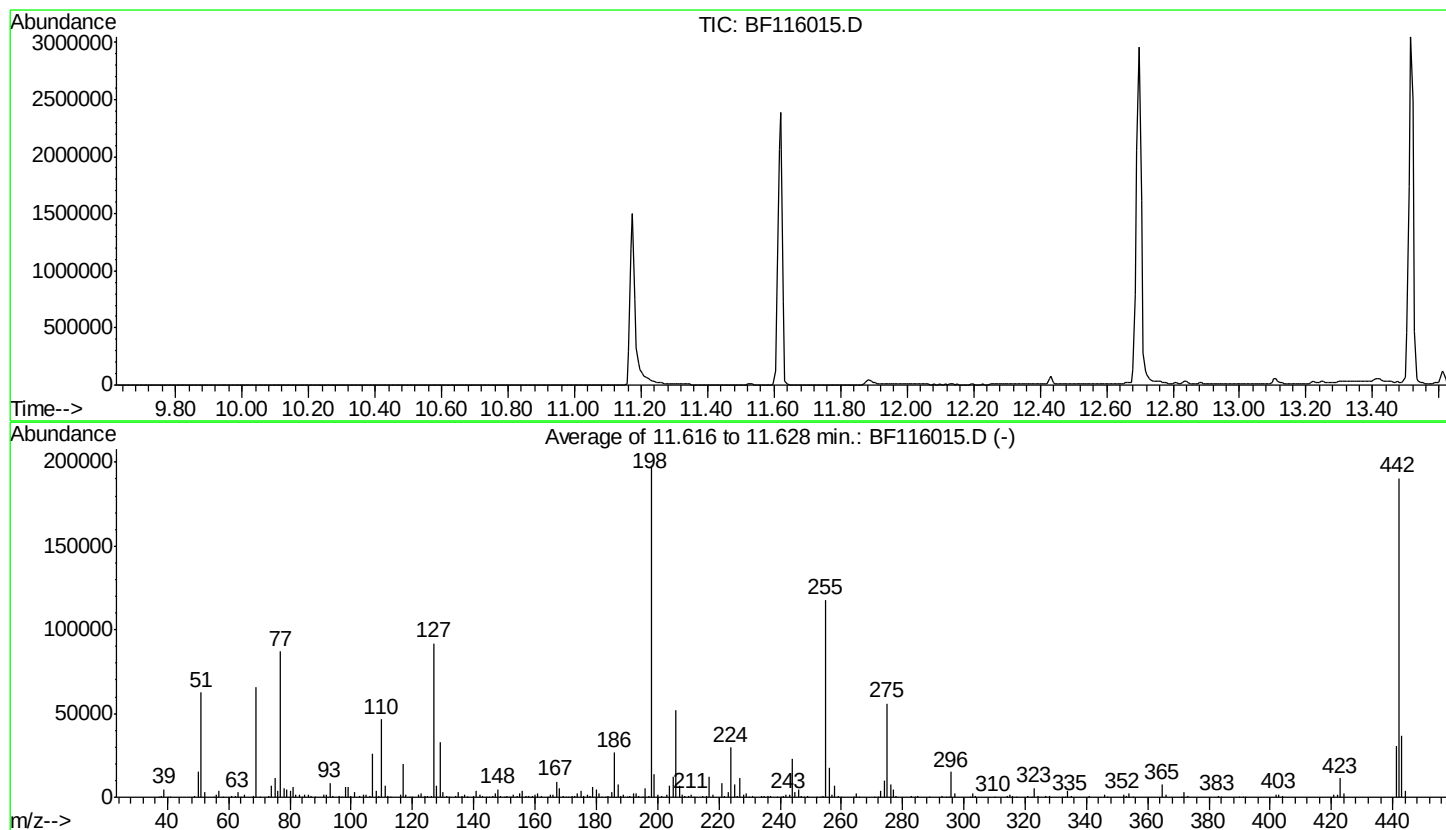

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	62421	PASS
68	69	0.00	2	1.3	836	PASS
69	198	0.00	100	33.3	65934	PASS
70	69	0.00	2	0.5	323	PASS
127	198	10	80	46.5	92053	PASS
197	198	0.00	2	0.6	1169	PASS
198	198	100	100	100.0	198018	PASS
199	198	5	9	6.9	13712	PASS
275	198	10	60	28.2	55925	PASS
365	198	1	100	3.7	7416	PASS
441	198	0.01	100	15.4	30469	PASS
442	198	50	100	96.3	190634	PASS
443	442	15	24	19.3	36800	PASS