
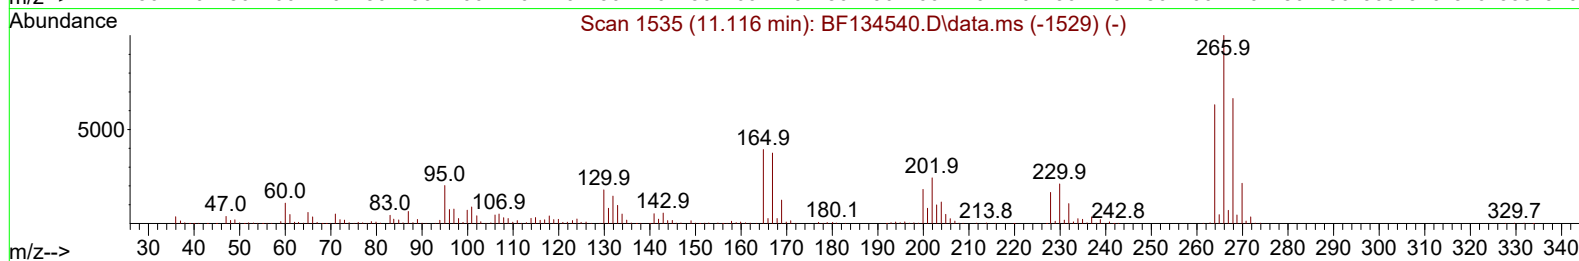
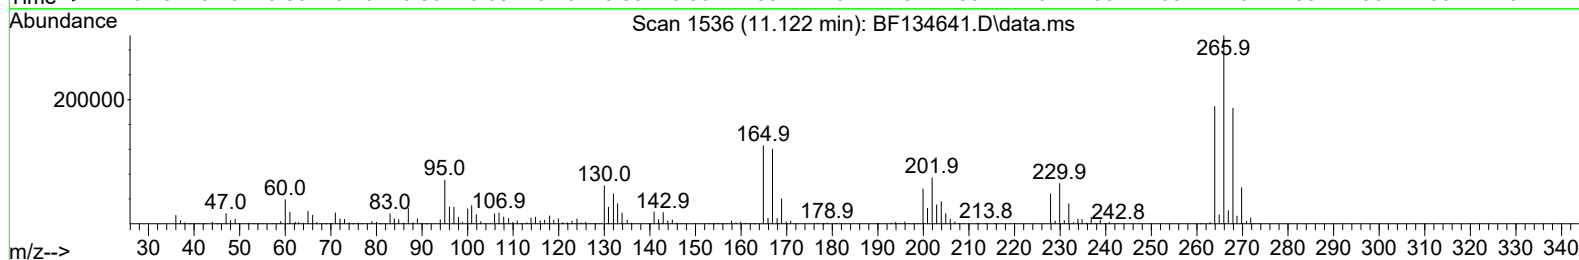


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\
Data File : BF134641.D
Acq On : 07 Aug 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 09:08:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

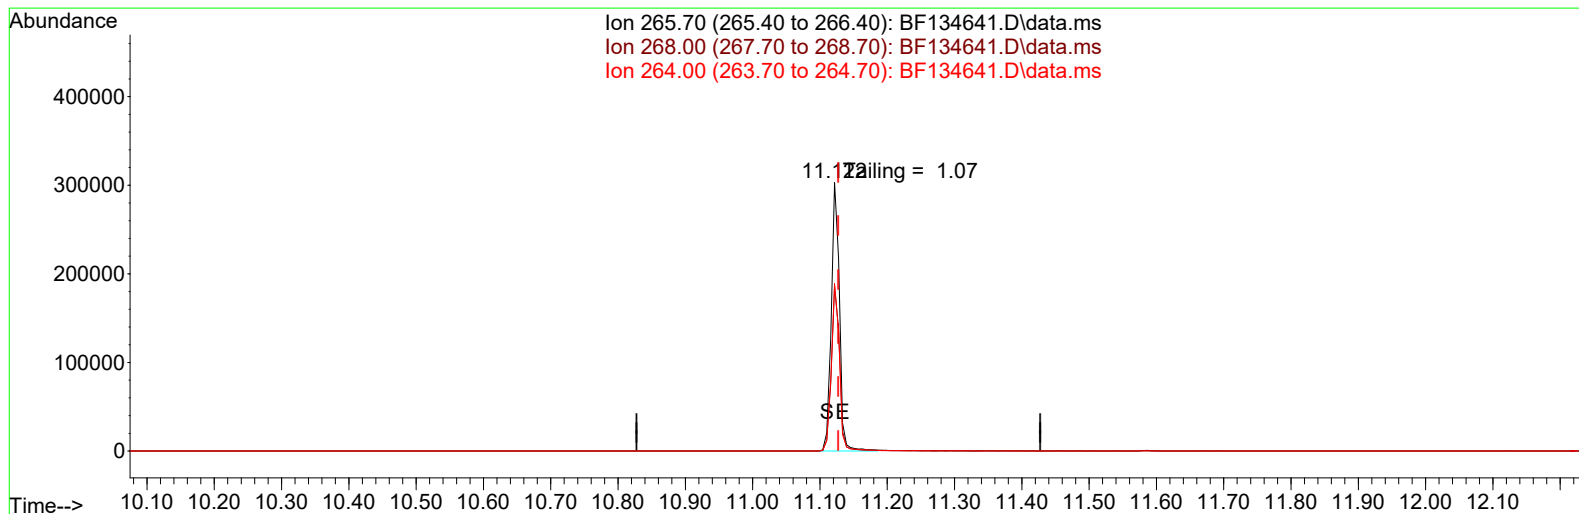

TIC: BF134641.D\data.ms

(70) Pentachlorophenol (C)




11.122min (-0.006) 31590.53 ng

response 257307

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	61.34
264.00	59.70	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\
Data File : BF134641.D
Acq On : 07 Aug 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 09:08:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

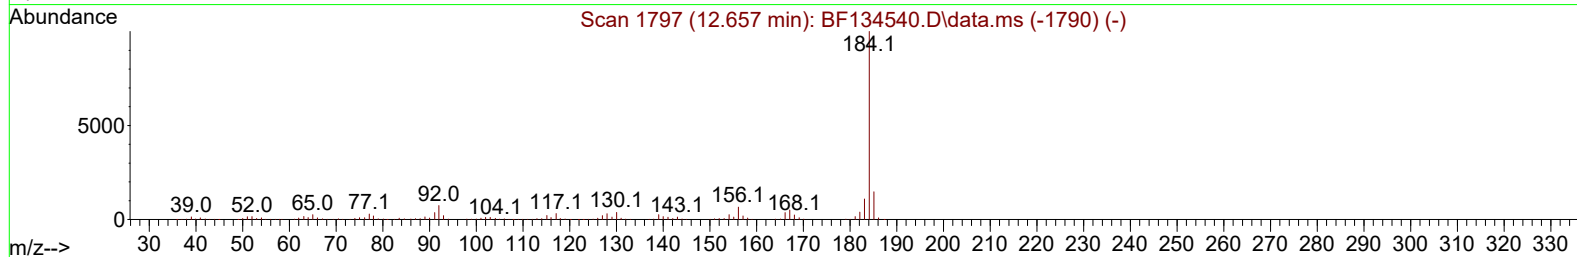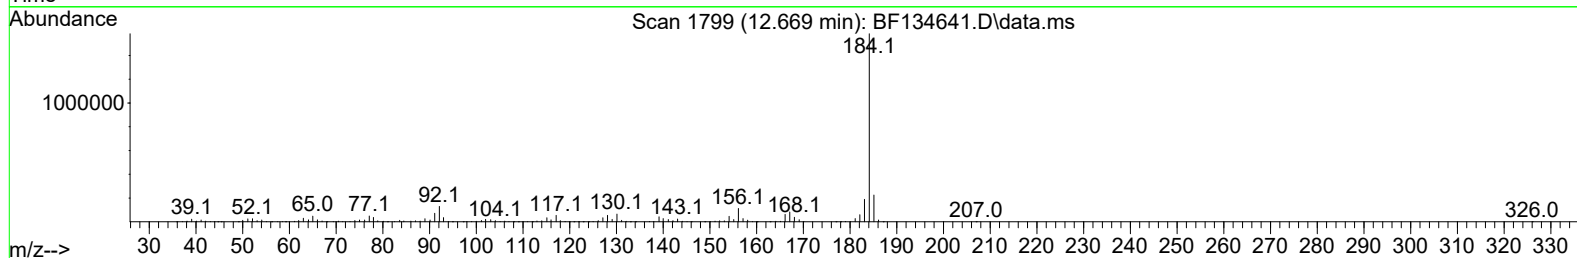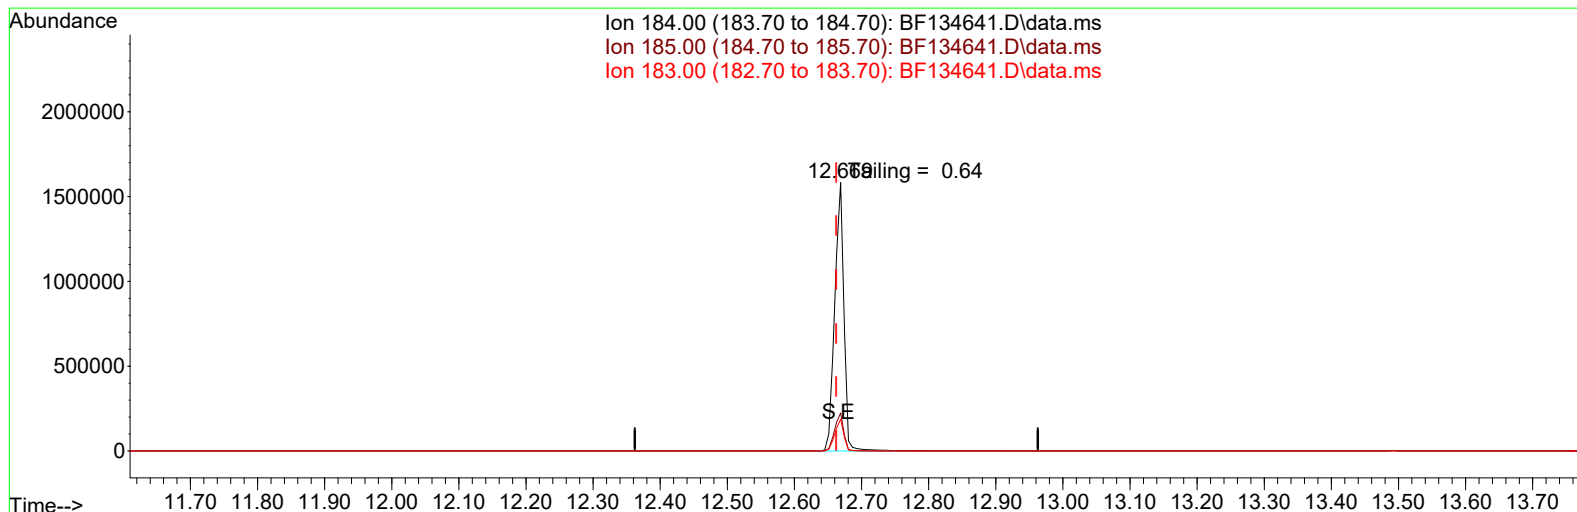

TIC: BF134641.D\data.ms

(77) Benzidine**12.669min (+ 0.006) 1119310.96 ng****response 1482170**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.23
183.00	10.80	11.91
0.00	0.00	0.00