

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\
 Data File : BF134653.D
 Acq On : 07 Aug 2023 14:37
 Operator : CG\JU
 Sample : 03887-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MCLEAN-TP7

Quant Time: Aug 08 01:21:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 04 09:29:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.798	152	216350	20.000	ng	0.00
21) Naphthalene-d8	8.075	136	824565	20.000	ng	# 0.00
39) Acenaphthene-d10	9.834	164	384447	20.000	ng	0.00
64) Phenanthrene-d10	11.322	188	585936	20.000	ng	# 0.00
76) Chrysene-d12	13.969	240	450343	20.000	ng	# 0.00
86) Perylene-d12	15.439	264	449756	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	1036698	72.840	ng	0.00
7) Phenol-d6	6.434	99	1278320	70.262	ng	0.00
23) Nitrobenzene-d5	7.357	82	739559	56.050	ng	-0.01
42) 2,4,6-Tribromophenol	10.622	330	266398	67.975	ng	0.00
45) 2-Fluorobiphenyl	9.151	172	1230738	53.228	ng	-0.01
79) Terphenyl-d14	12.916	244	1101945	43.136	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\
Data File : BF134653.D
Acq On : 07 Aug 2023 14:37
Operator : CG\JU
Sample : 03887-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MCLEAN-TP7

Quant Time: Aug 08 01:21:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration




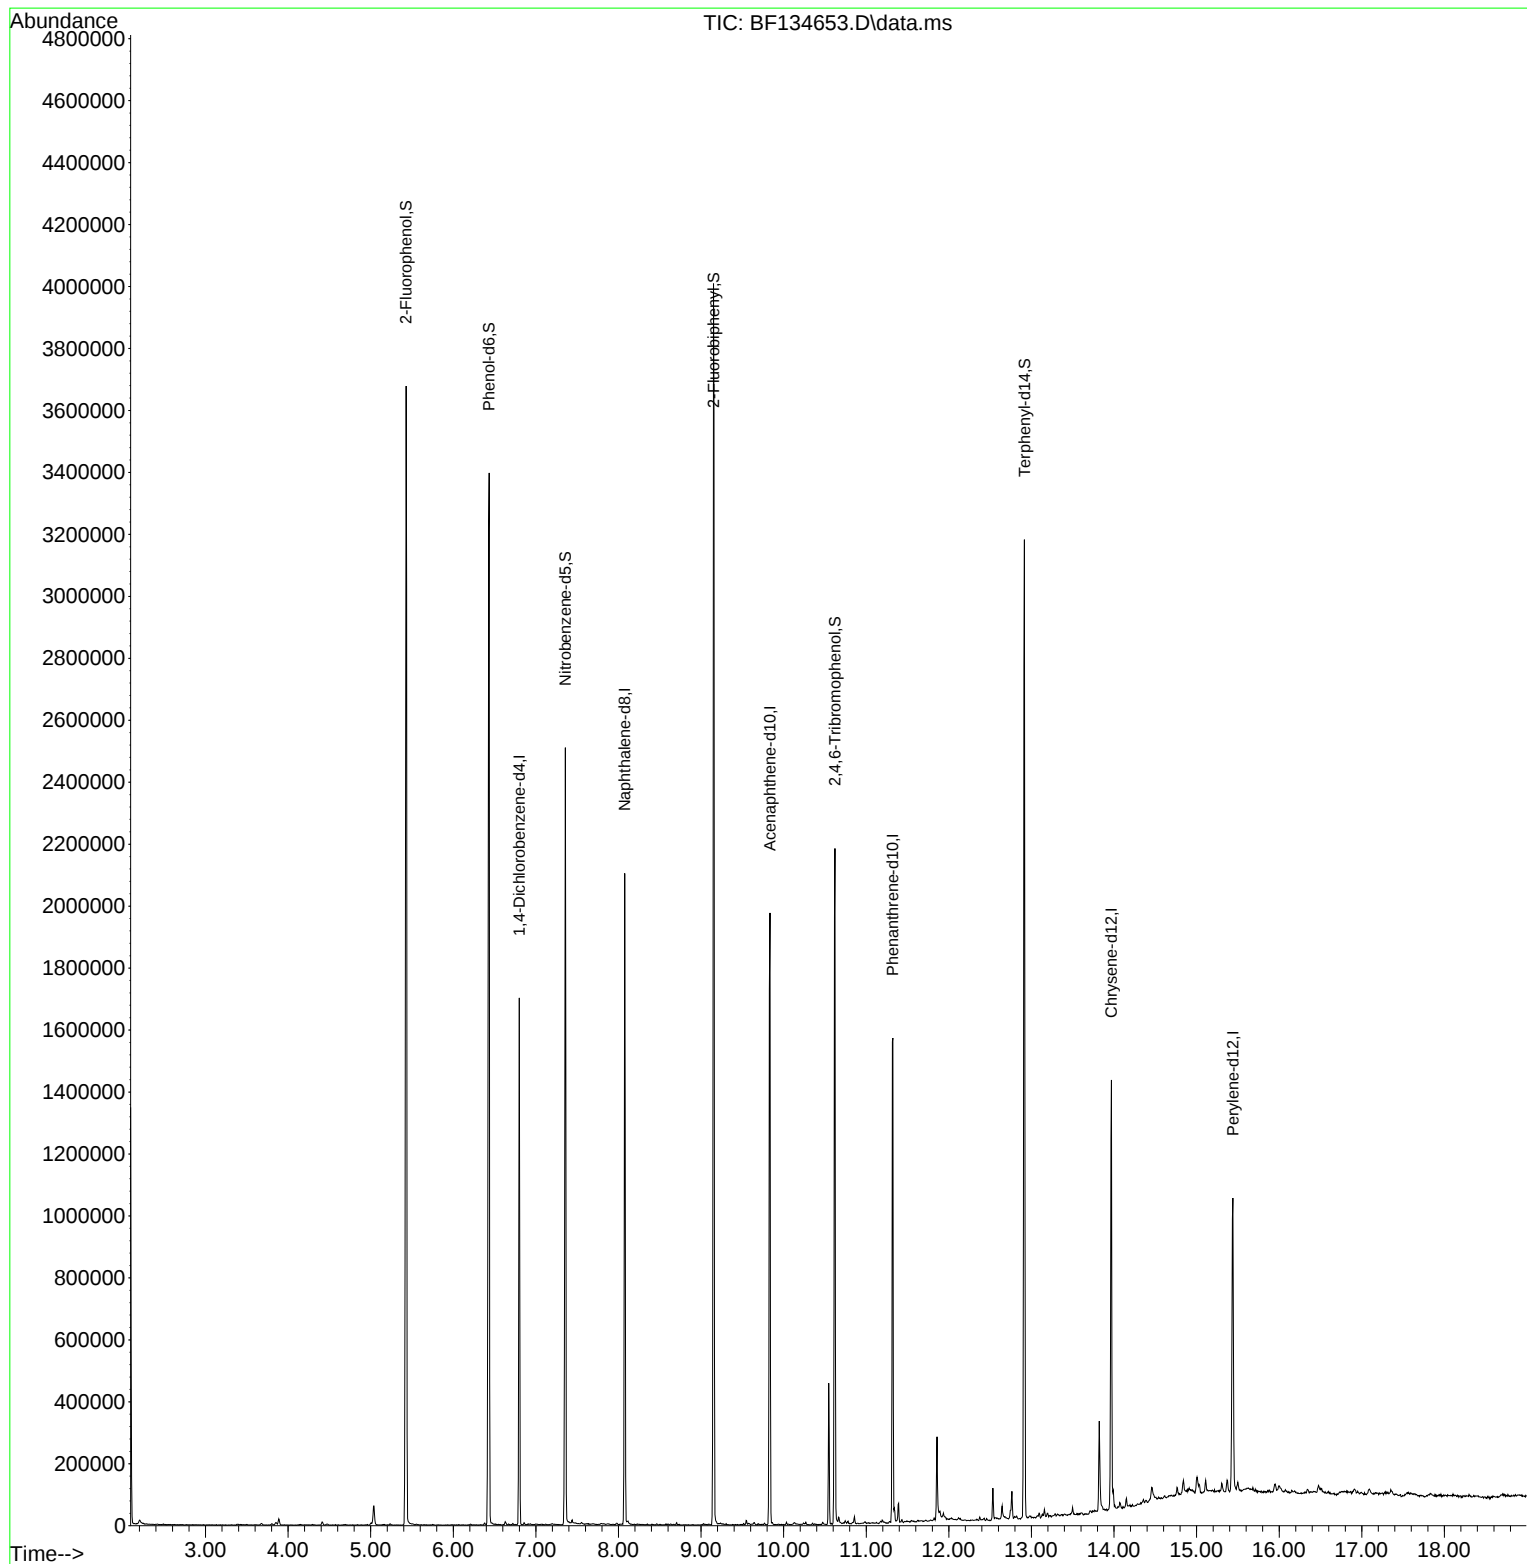


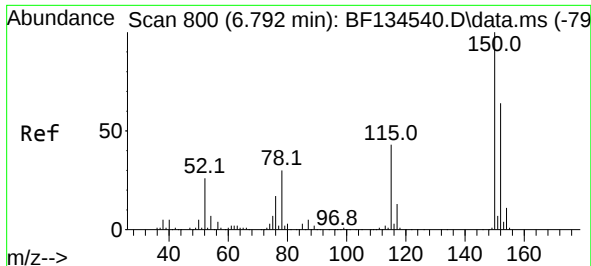

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.798 min Scan# 800
 Delta R.T. 0.000 min
 Lab File: BF134653.D
 Acq: 07 Aug 2023 14:37




Instrument :
 BNA_F
 ClientSampleId :
 MCLEAN-TP7


Tgt Ion:152 Resp: 216350
 Ion Ratio Lower Upper
 152 100
 150 156.5 128.3 192.5
 115 63.2 52.4 78.6

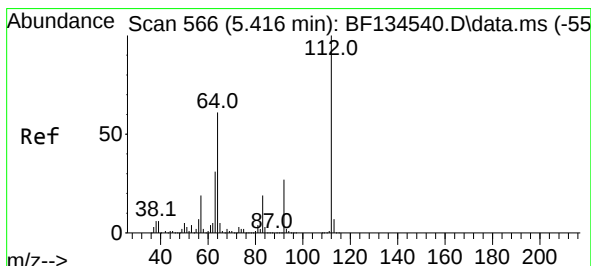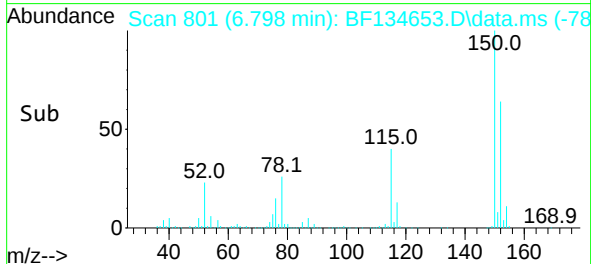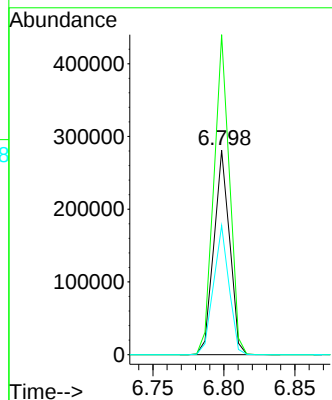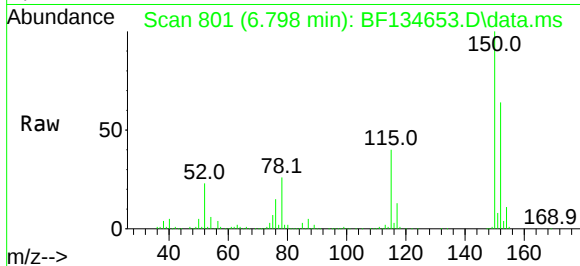

#5
 2-Fluorophenol
 Concen: 72.840 ng
 RT: 5.428 min Scan# 568
 Delta R.T. 0.000 min
 Lab File: BF134653.D
 Acq: 07 Aug 2023 14:37

Tgt Ion:112 Resp: 1036698
 Ion Ratio Lower Upper
 112 100
 64 62.4 44.9 67.3
 63 31.3 25.4 38.0


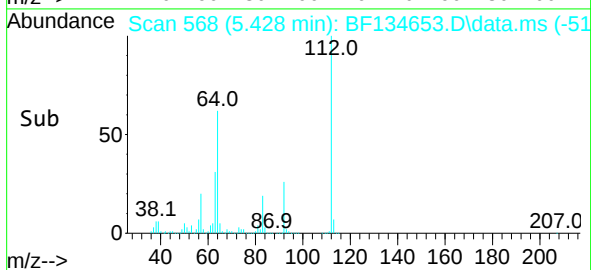
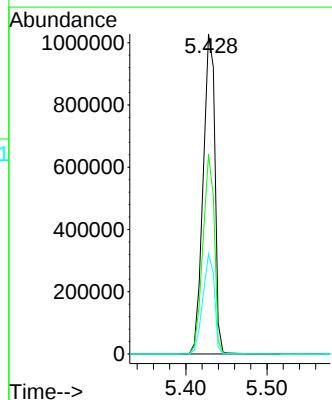
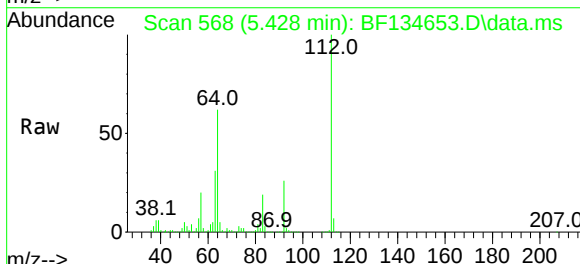


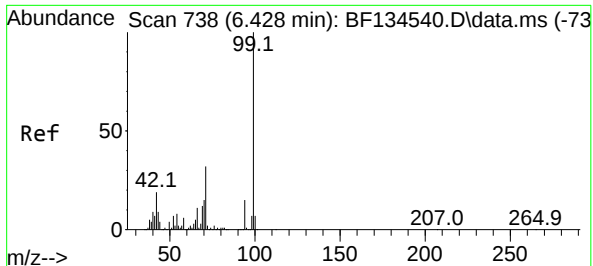

#7
Phenol-d6
Concen: 70.262 ng
RT: 6.434 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF134653.D
Acq: 07 Aug 2023 14:37




Instrument :
BNA_F
ClientSampleId :
MCLEAN-TP7

Tgt Ion: 99 Resp: 1278320
Ion Ratio Lower Upper
99 100
42 18.2 18.7 28.1#
71 32.2 36.4 54.6#

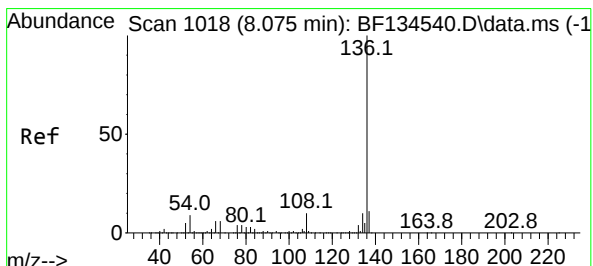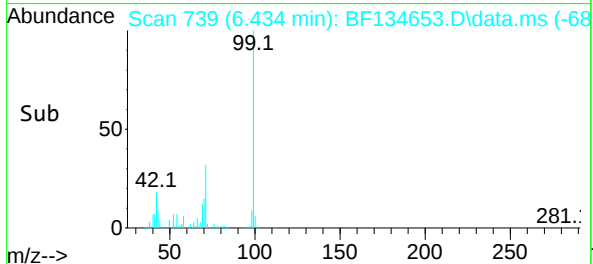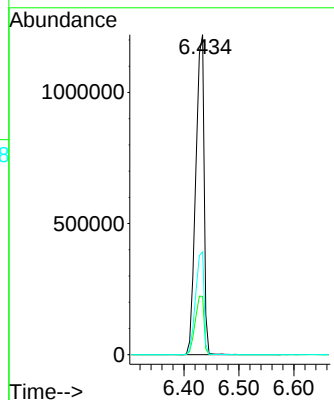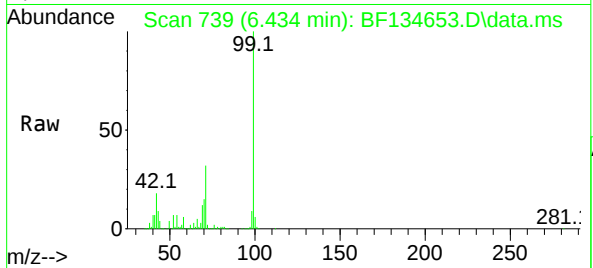

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.075 min Scan# 1018
Delta R.T. -0.006 min
Lab File: BF134653.D
Acq: 07 Aug 2023 14:37

Tgt Ion: 136 Resp: 824565
Ion Ratio Lower Upper
136 100
137 11.2 8.4 12.6
54 9.1 5.2 7.8#
68 6.8 2.9 4.3#

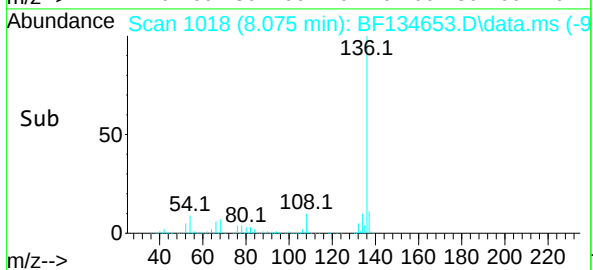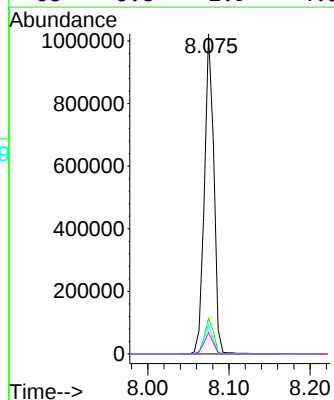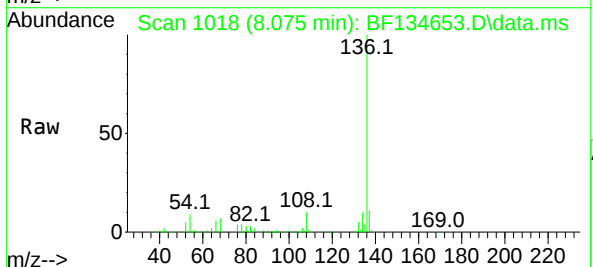



#23

Nitrobenzene-d5

Concen: 56.050 ng

RT: 7.357 min Scan# 896

Delta R.T. -0.012 min

Lab File: BF134653.D

Acq: 07 Aug 2023 14:37

Instrument :

BNA_F

ClientSampleId :

MCLEAN-TP7





Tgt Ion: 82 Resp: 739559

Ion Ratio Lower Upper

82 100

128 44.3 34.3 51.5

54 53.9 43.8 65.6

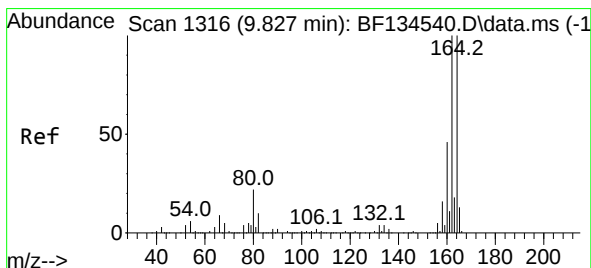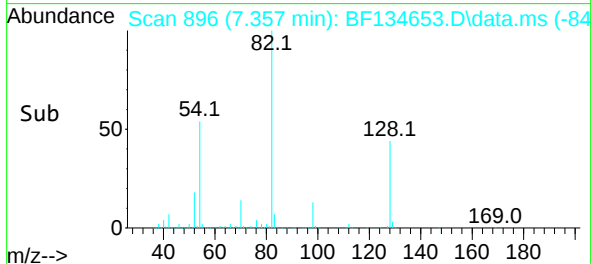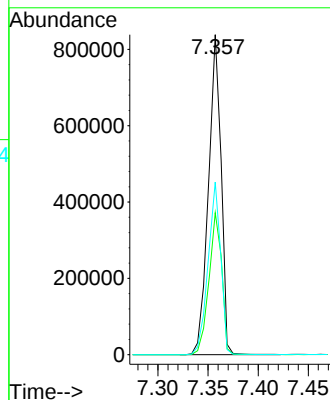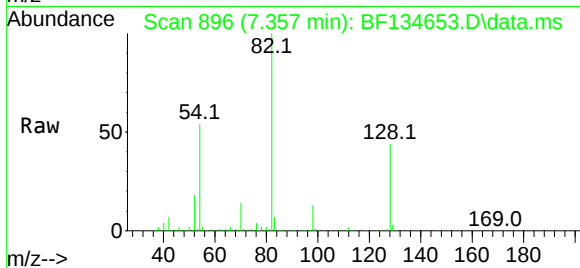

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.834 min Scan# 1317

Delta R.T. 0.000 min

Lab File: BF134653.D

Acq: 07 Aug 2023 14:37




Tgt Ion: 164 Resp: 384447


Ion Ratio Lower Upper

164 100

162 100.7 82.6 123.8

160 46.3 37.2 55.8

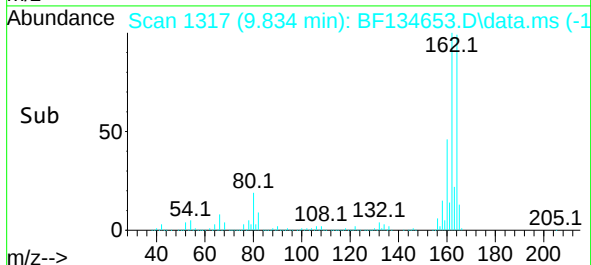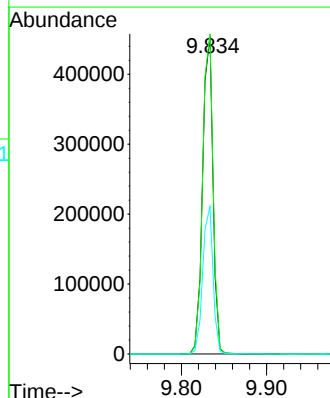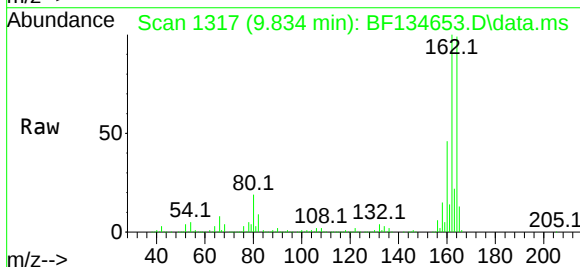

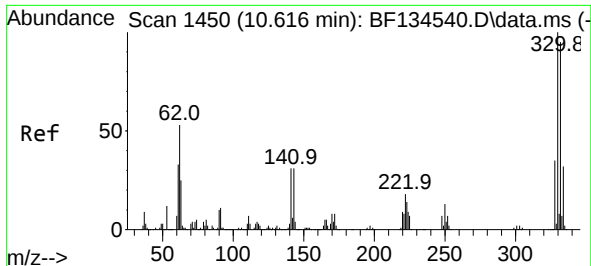

#42

2,4,6-Tribromophenol

Concen: 67.975 ng

RT: 10.622 min Scan# 1451

Delta R.T. -0.006 min

Lab File: BF134653.D


Acq: 07 Aug 2023 14:37

Instrument :

BNA_F

ClientSampleId :

MCLEAN-TP7

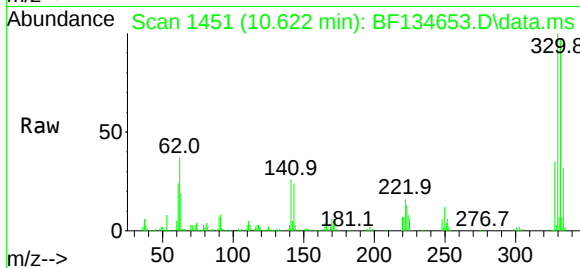




Tgt Ion:330 Resp: 266398

Ion Ratio Lower Upper

330 100

332 95.8 78.8 118.2

141 29.9 25.4 38.2

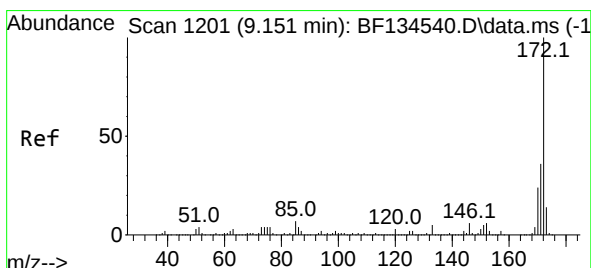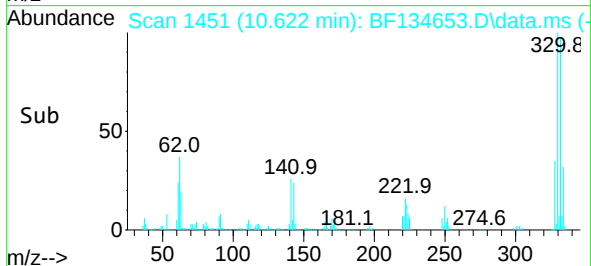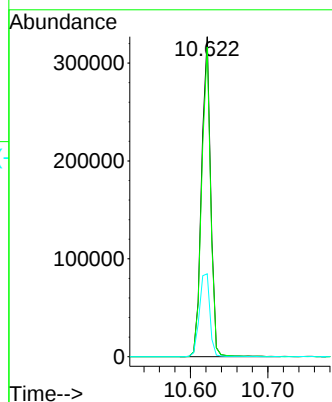

#45

2-Fluorobiphenyl

Concen: 53.228 ng

RT: 9.151 min Scan# 1201

Delta R.T. -0.012 min

Lab File: BF134653.D

Acq: 07 Aug 2023 14:37




Tgt Ion:172 Resp: 1230738


Ion Ratio Lower Upper

172 100

171 35.7 28.8 43.2

170 23.5 18.7 28.1


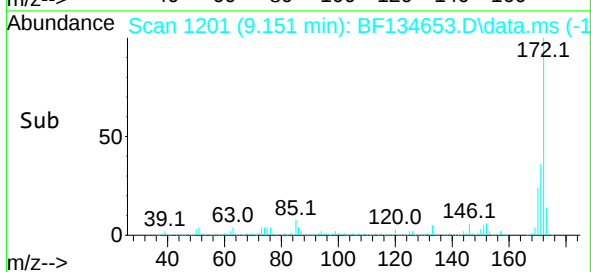
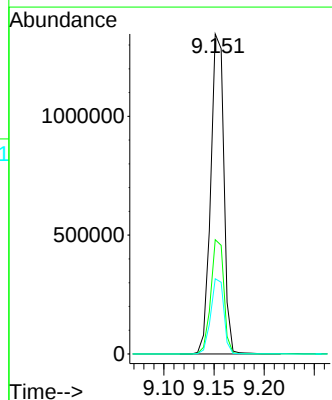
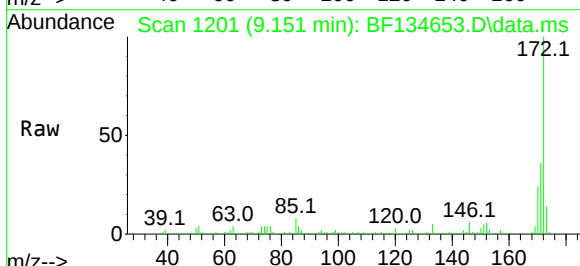


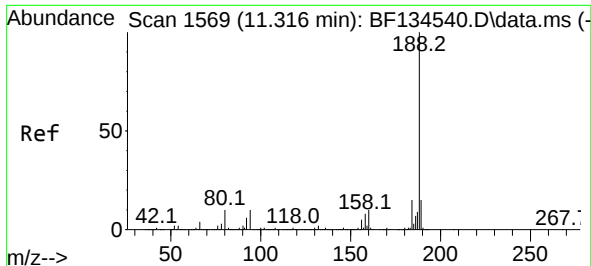

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.322 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF134653.D
Acq: 07 Aug 2023 14:37




Instrument :
BNA_F
ClientSampleId :
MCLEAN-TP7


Tgt Ion:188 Resp: 585936
Ion Ratio Lower Upper
188 100
94 8.7 5.1 7.7#
80 9.4 6.6 9.8

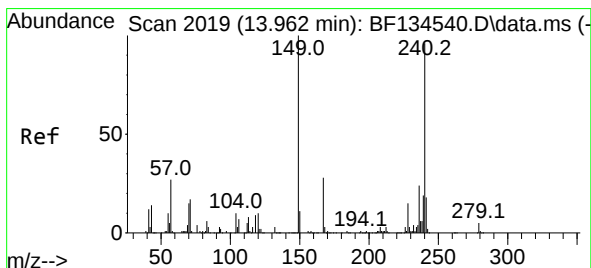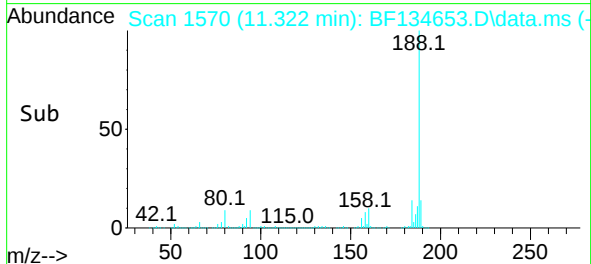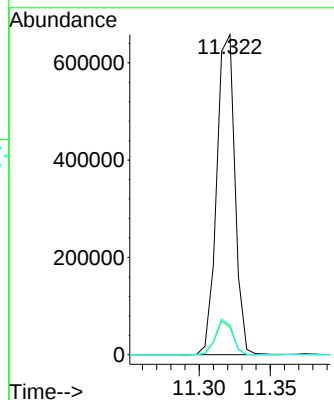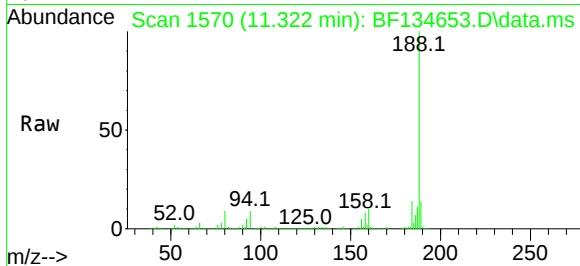

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.969 min Scan# 2020
Delta R.T. -0.006 min
Lab File: BF134653.D
Acq: 07 Aug 2023 14:37


Tgt Ion:240 Resp: 450343
Ion Ratio Lower Upper
240 100
120 10.2 6.6 10.0#
236 25.8 20.2 30.2

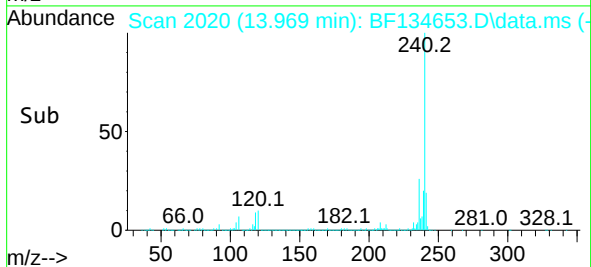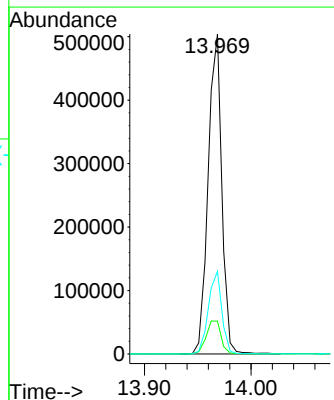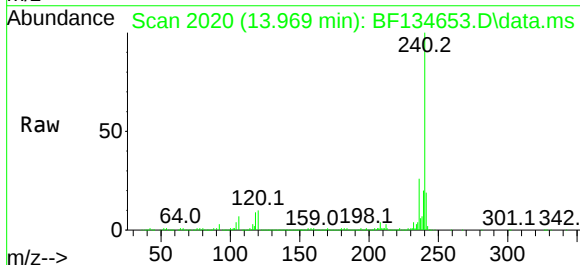



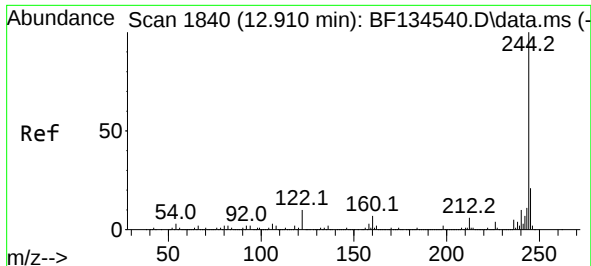


#79
 Terphenyl-d14
 Concen: 43.136 ng
 RT: 12.916 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF134653.D
 Acq: 07 Aug 2023 14:37

Instrument :
 BNA_F
 ClientSampleId :
 MCLEAN-TP7

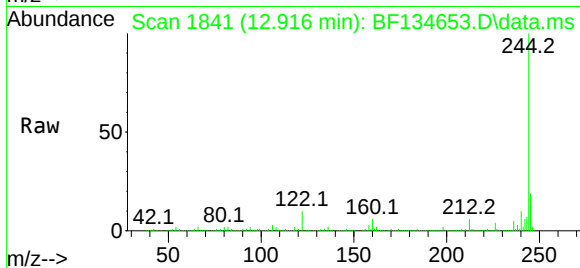

Tgt Ion:244 Resp: 1101945
 Ion Ratio Lower Upper
 244 100
 212 6.2 5.6 8.4
 122 10.0 8.0 12.0

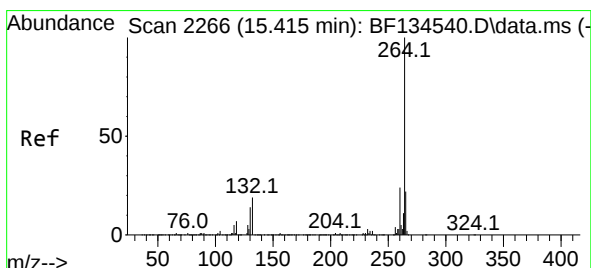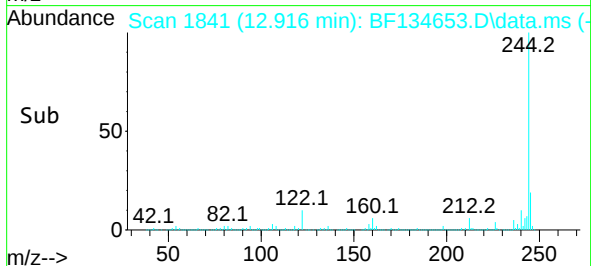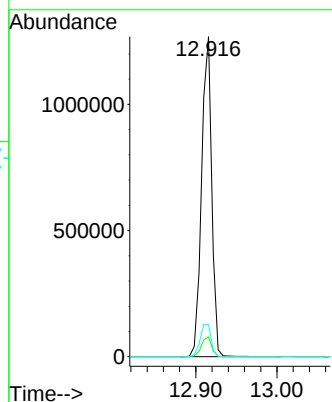

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.439 min Scan# 2270
 Delta R.T. 0.000 min
 Lab File: BF134653.D
 Acq: 07 Aug 2023 14:37

Tgt Ion:264 Resp: 449756
 Ion Ratio Lower Upper
 264 100
 260 23.9 18.4 27.6
 265 21.9 15.8 23.8

