

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\
 Data File : BF134658.D
 Acq On : 07 Aug 2023 17:21
 Operator : CG\JU
 Sample : 03903-08 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-08

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.863	292	302	308	rBV2	17881	29310	1.85%	0.237%
2	5.016	495	498	501	rBV	23619	24986	1.58%	0.202%
3	5.287	538	544	549	rBV	37580	35690	2.26%	0.289%
4	5.393	556	562	563	rBV	54899	51281	3.24%	0.415%
5	5.416	563	566	570	rVB	920220	747588	47.30%	6.056%
6	6.328	718	721	723	rBV	41273	32352	2.05%	0.262%
7	6.357	723	726	730	rVB	29059	22045	1.39%	0.179%
8	6.422	730	737	740	rBV	964026	745987	47.20%	6.043%
9	6.622	768	771	778	rBV	99928	82161	5.20%	0.666%
10	6.798	797	801	804	rBV	1582079	1252358	79.23%	10.146%
11	7.351	886	895	902	rBV	542512	428911	27.14%	3.475%
12	8.075	1014	1018	1021	rBV	2013003	1580604	100.00%	12.805%
13	9.151	1197	1201	1204	rBV	957308	751267	47.53%	6.086%
14	9.269	1218	1221	1226	rBV	26277	20252	1.28%	0.164%
15	9.828	1313	1316	1320	rBV	1743122	1535471	97.14%	12.439%
16	10.616	1446	1450	1458	rBV	438427	348574	22.05%	2.824%
17	11.316	1566	1569	1573	rBV	1438557	1287325	81.45%	10.429%
18	11.375	1575	1579	1586	rVB8	10191	26051	1.65%	0.211%
19	11.651	1624	1626	1632	rBV6	14783	24187	1.53%	0.196%
20	11.851	1657	1660	1664	rBV3	30087	26109	1.65%	0.212%
21	12.204	1714	1720	1722	rBV7	9758	21169	1.34%	0.171%
22	12.316	1734	1739	1742	rBV5	15998	27431	1.74%	0.222%
23	12.375	1746	1749	1751	rBV3	20373	20045	1.27%	0.162%
24	12.533	1773	1776	1779	rBV	26541	27897	1.76%	0.226%
25	12.639	1791	1794	1797	rBV5	15367	19511	1.23%	0.158%
26	12.763	1812	1815	1818	rBV	33185	32993	2.09%	0.267%
27	12.827	1823	1826	1829	rBV3	26465	31363	1.98%	0.254%
28	12.910	1836	1840	1849	rBV	676032	569616	36.04%	4.615%
29	13.286	1902	1904	1907	rVB2	36708	30933	1.96%	0.251%
30	13.322	1907	1910	1912	rBV	26715	28441	1.80%	0.230%
31	13.357	1914	1916	1920	rBV4	29264	33132	2.10%	0.268%
32	13.392	1920	1922	1927	rBV5	31306	48731	3.08%	0.395%
33	13.704	1972	1975	1977	rBV4	43452	62072	3.93%	0.503%
34	13.963	2016	2019	2023	rBV	1319287	1287707	81.47%	10.432%
35	15.433	2265	2269	2274	rVB	867583	1050347	66.45%	8.509%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\
Data File : BF134658.D
Acq On : 07 Aug 2023 17:21
Operator : CG\JU
Sample : 03903-08 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-08

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 12343897

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\
Data File : BF134658.D
Acq On : 07 Aug 2023 17:21
Operator : CG\JU
Sample : 03903-08 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

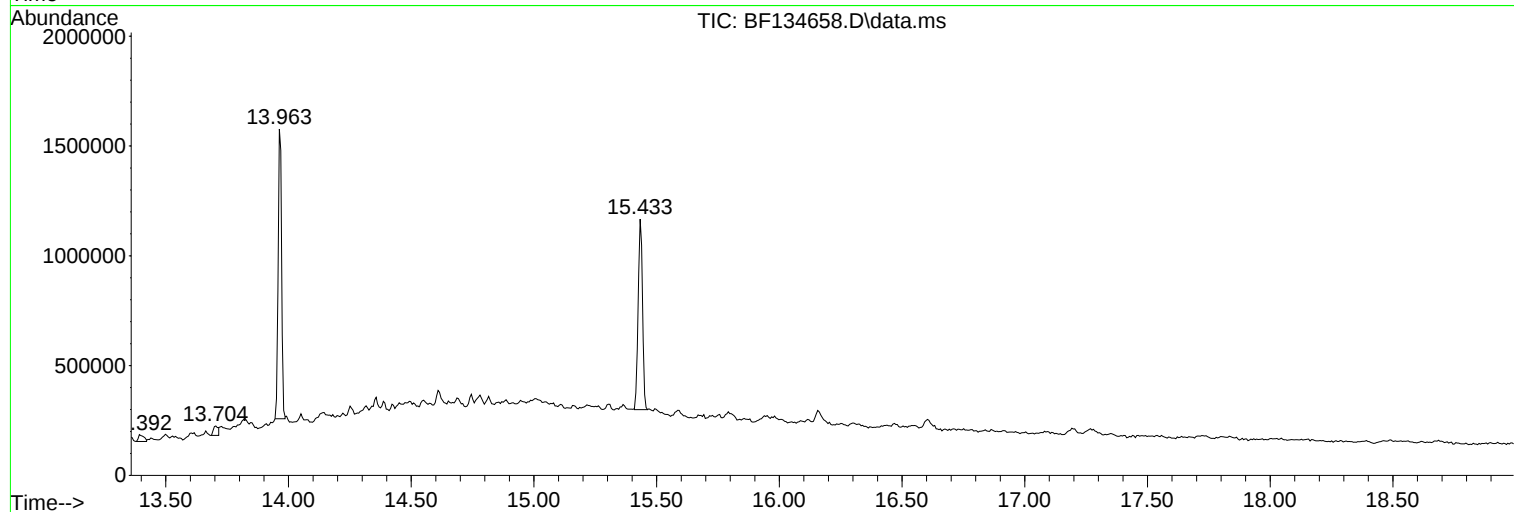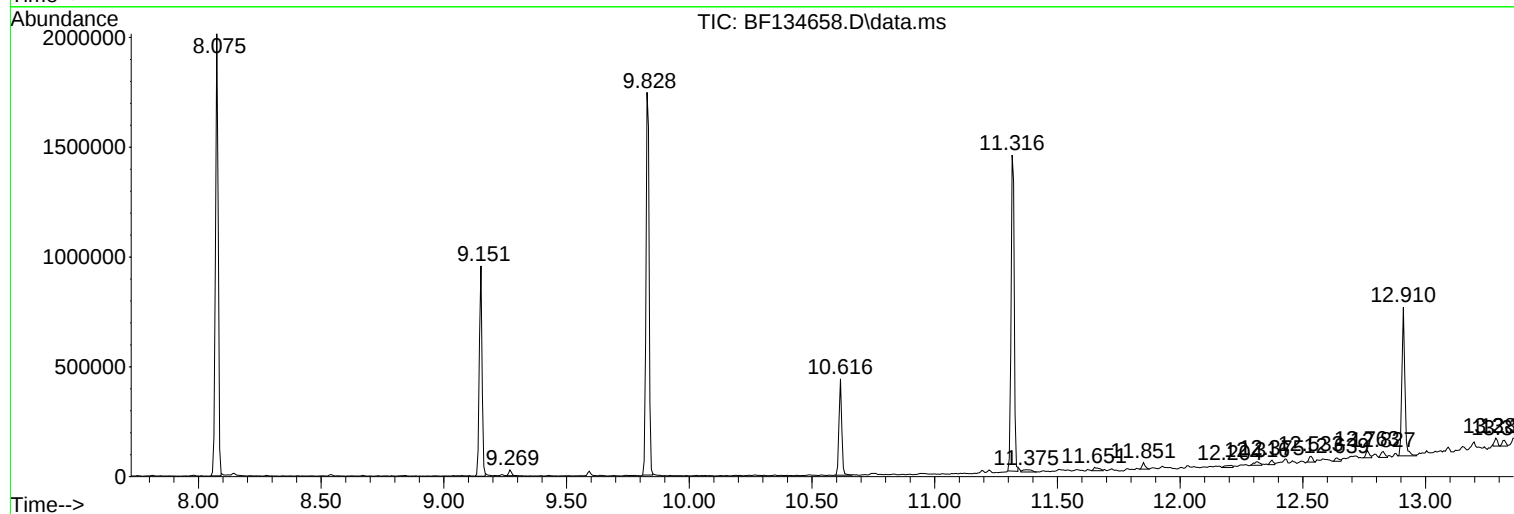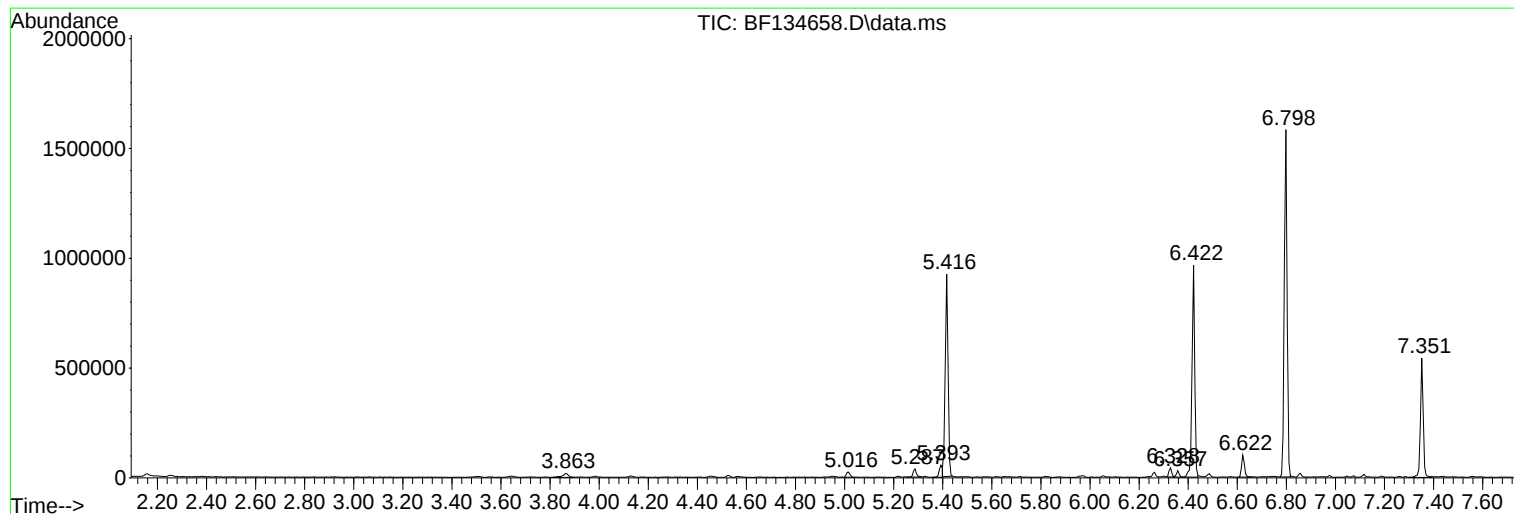

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\
Data File : BF134658.D
Acq On : 07 Aug 2023 17:21
Operator : CG\JU
Sample : 03903-08 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\
Data File : BF134658.D
Acq On : 07 Aug 2023 17:21
Operator : CG\JU
Sample : 03903-08 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------