


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\
Data File : BF134641.D
Acq On : 07 Aug 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 04 09:29:15 2023

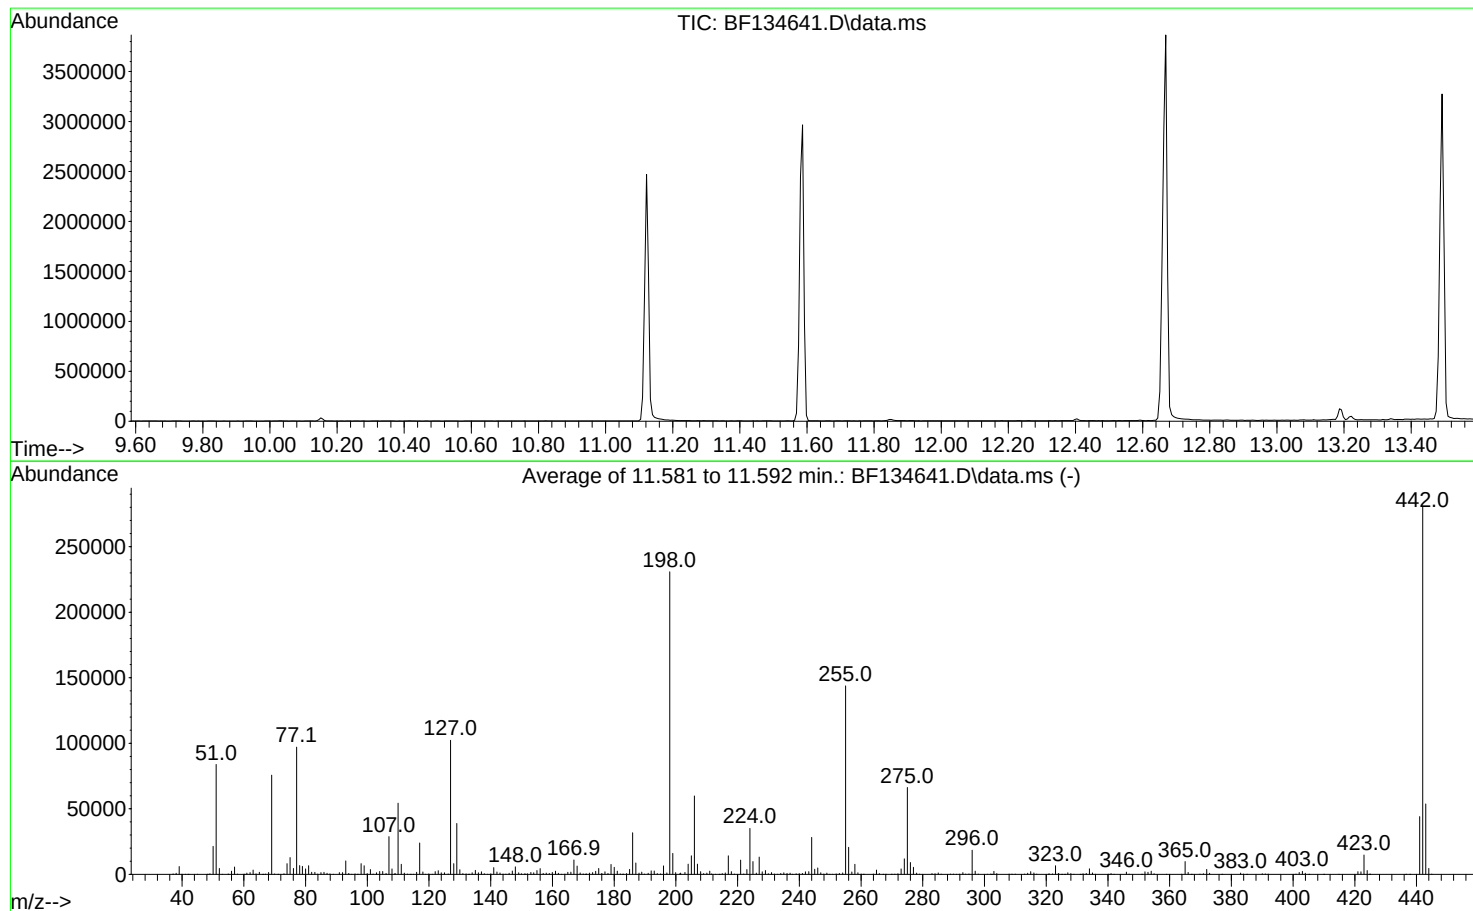




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	83835	PASS
68	69	0.00	2	1.9	1423	PASS
69	198	0.00	100	32.8	75755	PASS
70	69	0.00	2	0.6	430	PASS
127	198	10	80	44.3	102261	PASS
197	198	0.00	2	0.5	1091	PASS
198	198	100	100	100.0	230824	PASS
199	198	5	9	6.9	15972	PASS
275	198	10	60	28.7	66341	PASS
365	198	1	100	4.2	9744	PASS
441	198	0.01	100	19.1	44053	PASS
442	442	50	100	100.0	280661	PASS
443	442	15	24	19.1	53696	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\
 Data File : BF134641.D
 Acq On : 07 Aug 2023 08:10
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 07 09:08:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 04 09:29:15 2023
 Response via : Initial Calibration

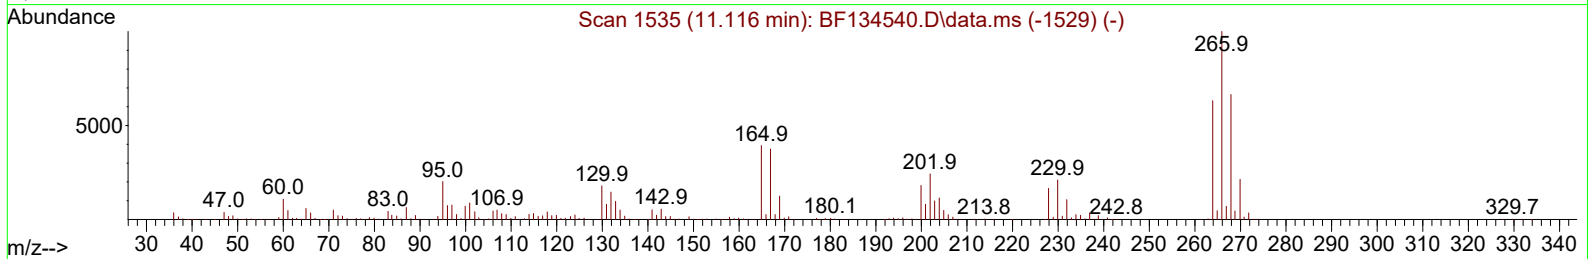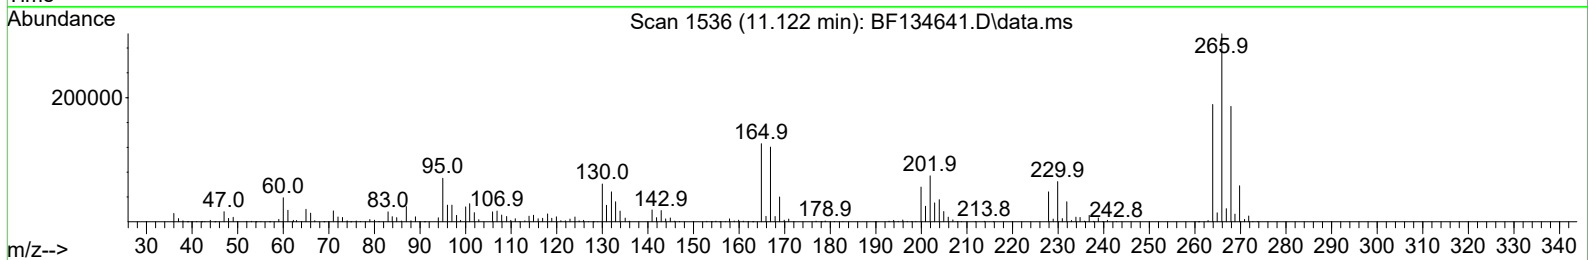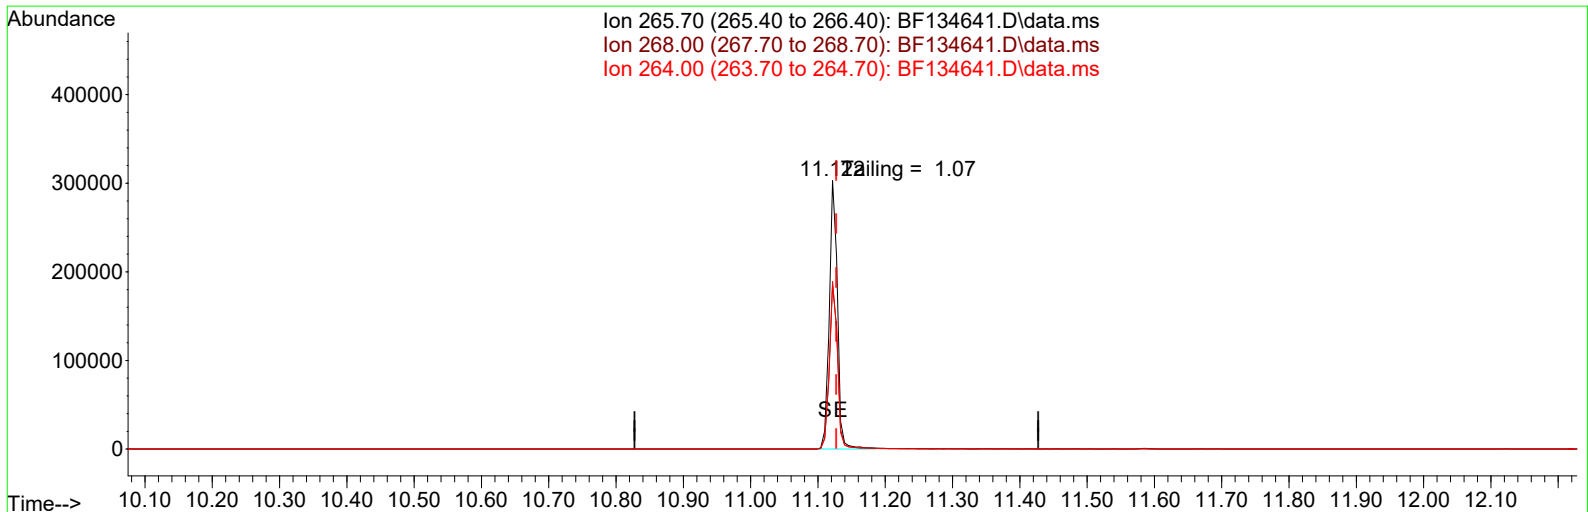

TIC: BF134641.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.006) 31590.53 ng




response 257307

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	61.34
264.00	59.70	62.38
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080723\  
Data File : BF134641.D  
Acq On    : 07 Aug 2023  08:10  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 07 09:08:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

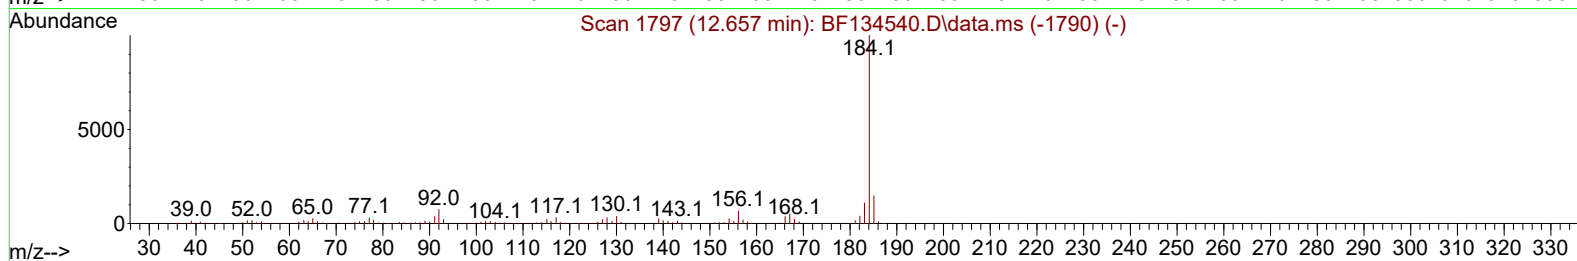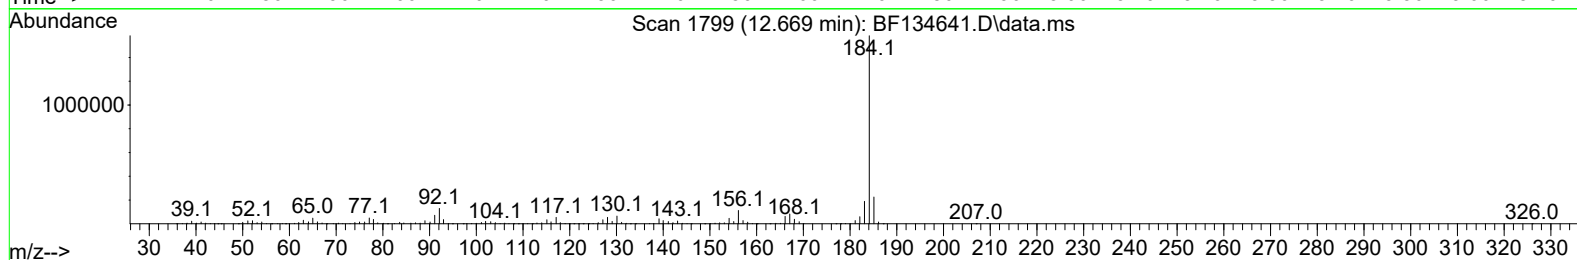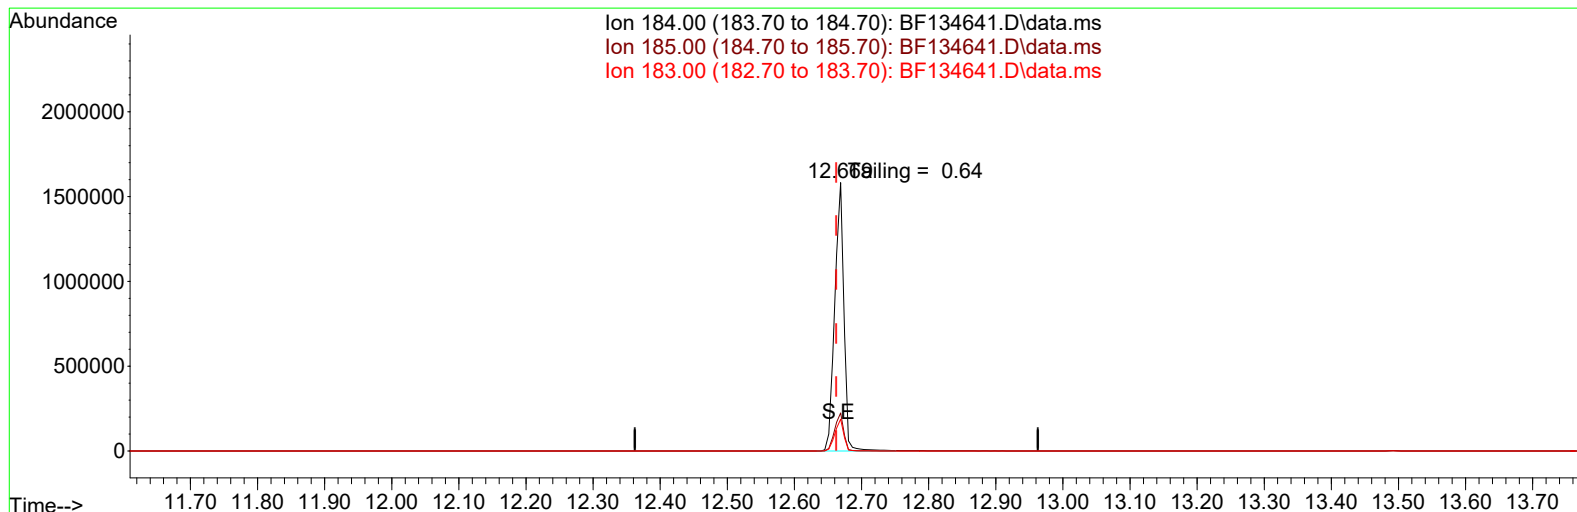

TIC: BF134641.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 1119310.96 ng

response **1482170**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.00	14.23
--------	-------	-------

183.00	10.80	11.91
--------	-------	-------

0.00 0.00 0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/7/2023	BNA_F	<u>BF134641.D</u>
Compound Name	Response	Retention Time
DDT	536945	13.492
DDD	24156	13.186
DDE	306	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24462	561407	4.36

Instrument :
BNA_F
ClientSampleId :
DFTPP