



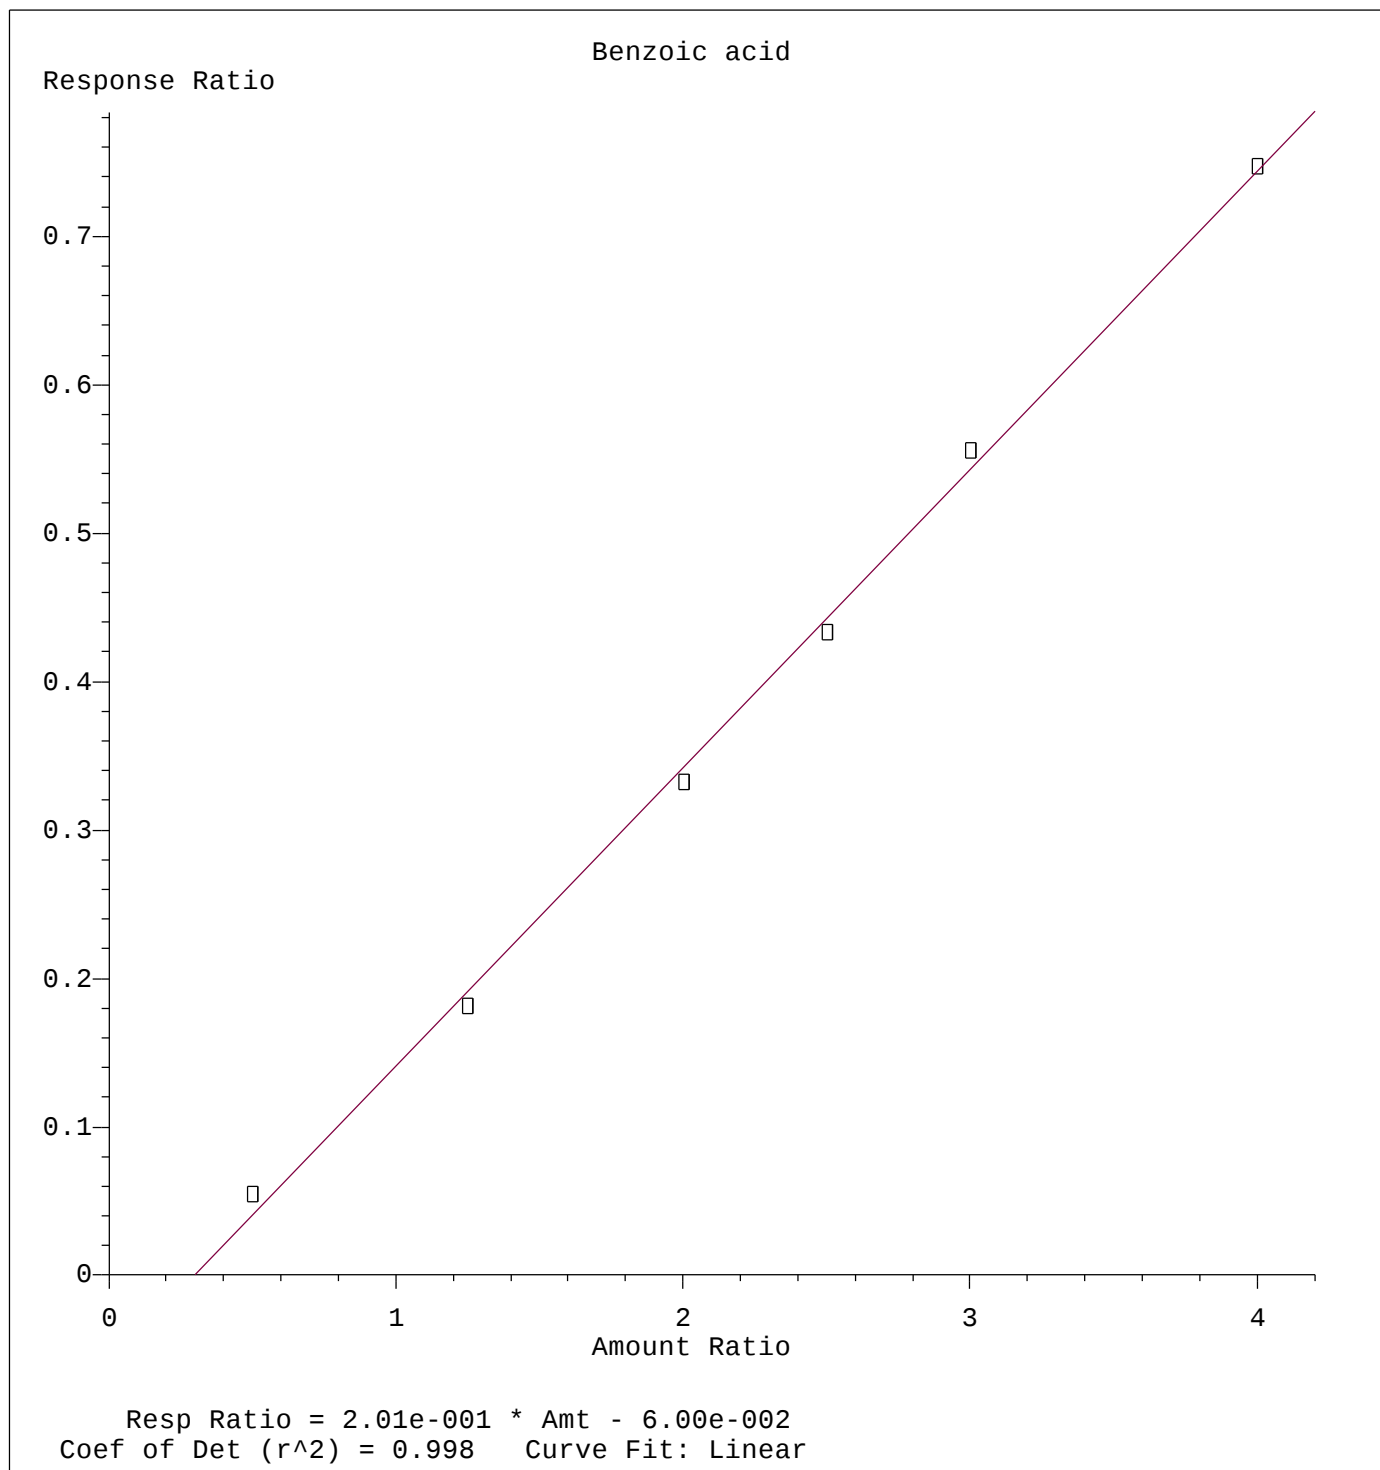


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Calibration Table Last Updated: Wed Aug 08 12:24:24 2018

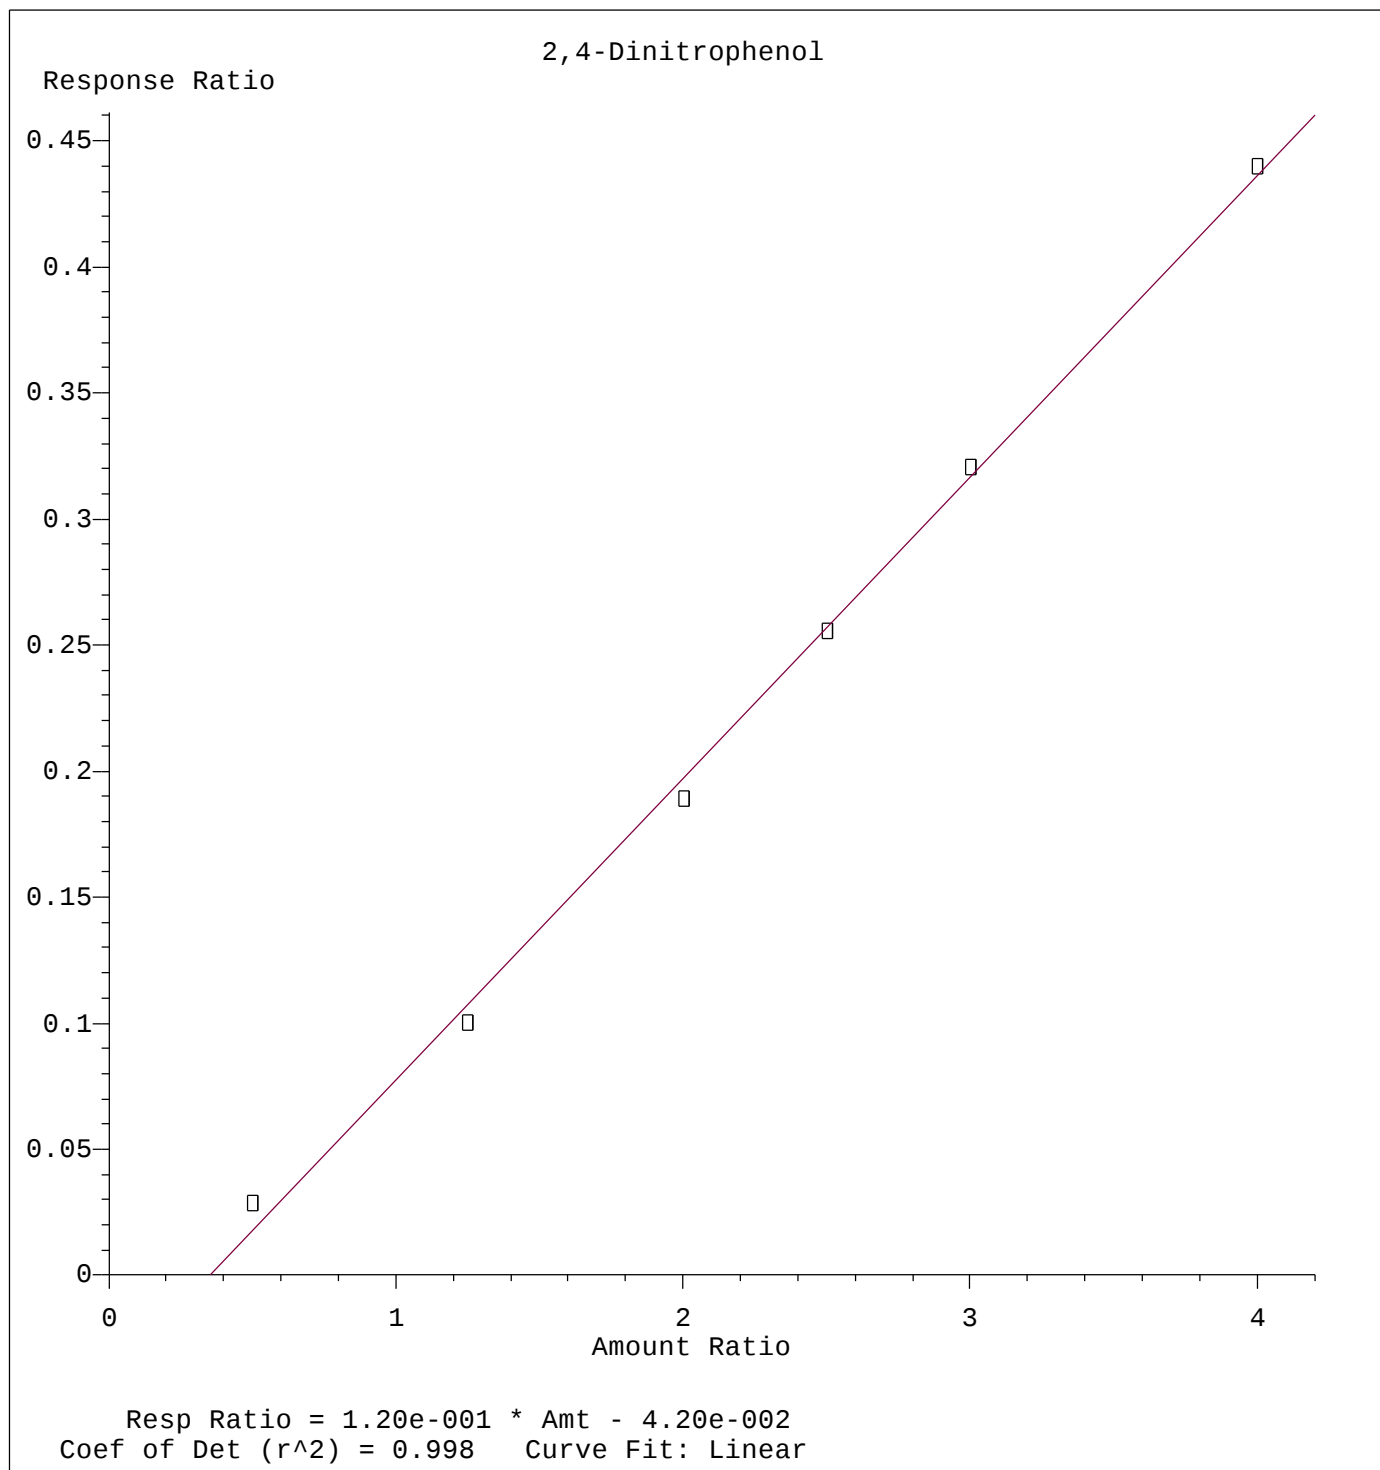

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Calibration Table Last Updated: Wed Aug 08 12:24:24 2018

4,6-Dinitro-2-methylphenol

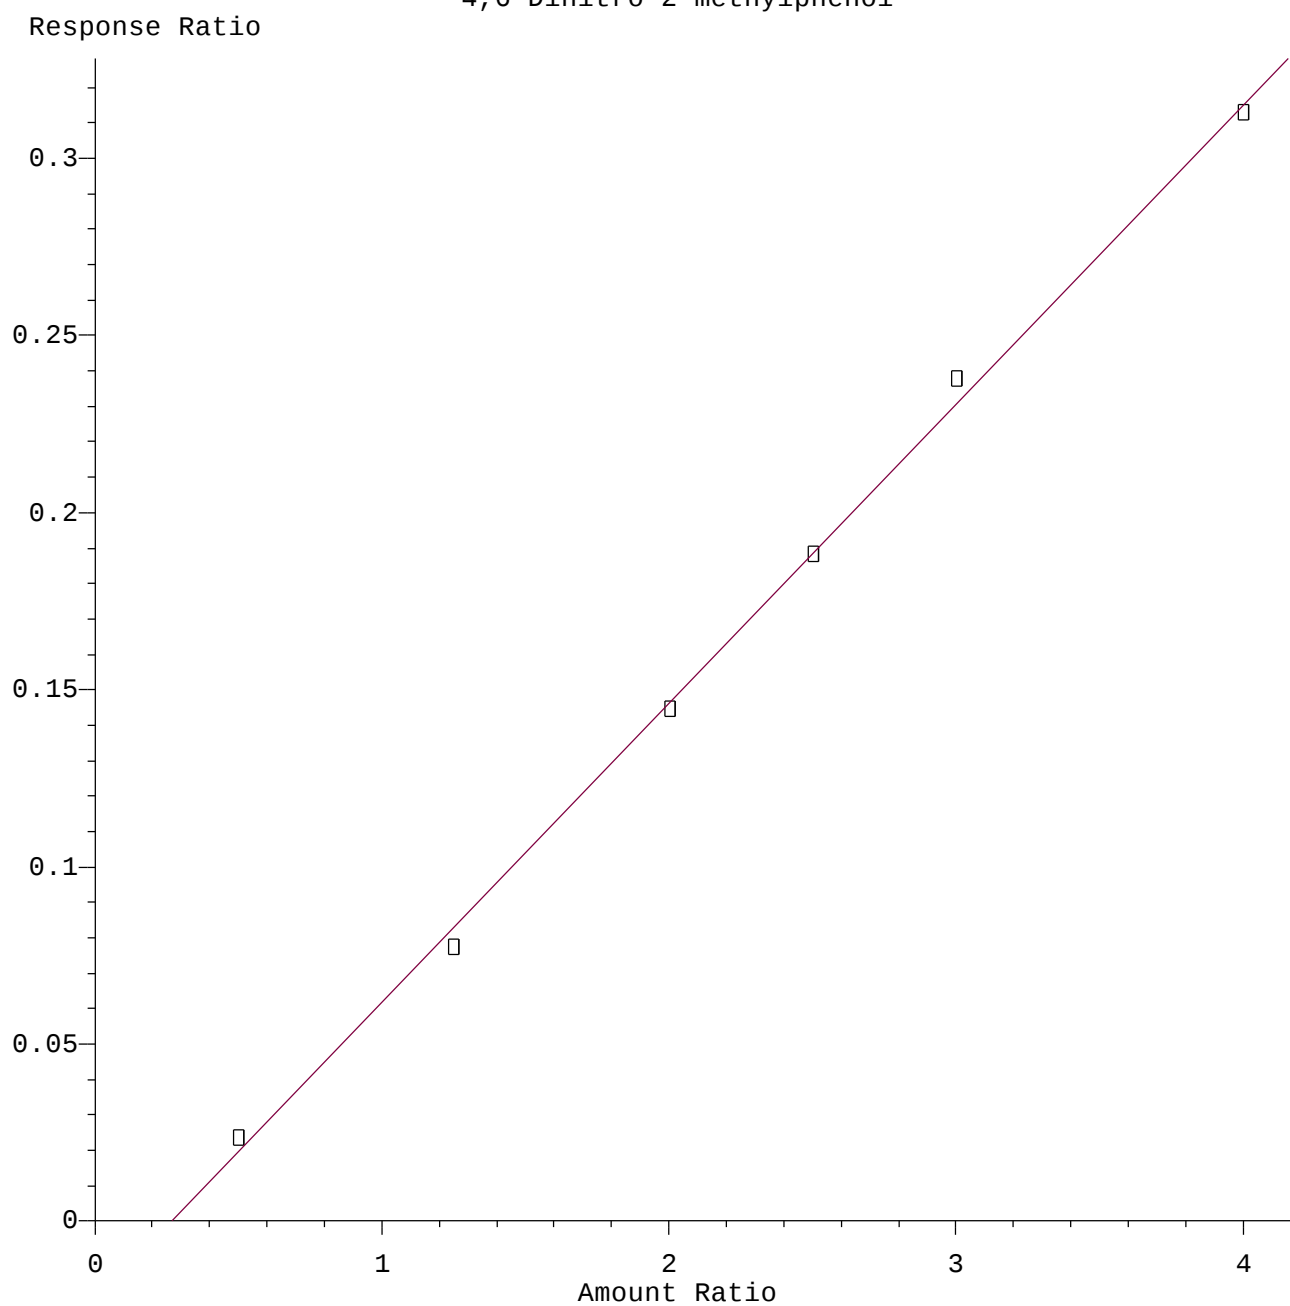

Resp Ratio = 8.45×10^{-2} * Amt - 2.26×10^{-2}
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Calibration Table Last Updated: Wed Aug 08 12:24:24 2018