
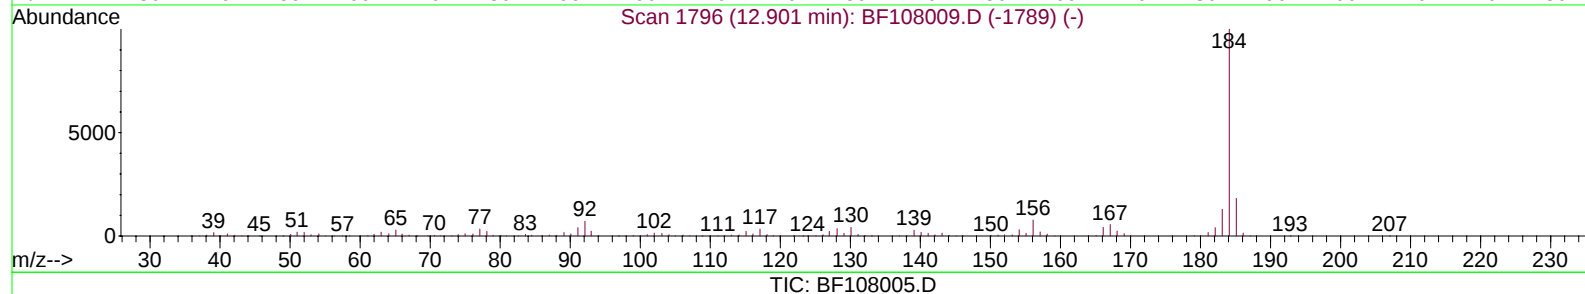
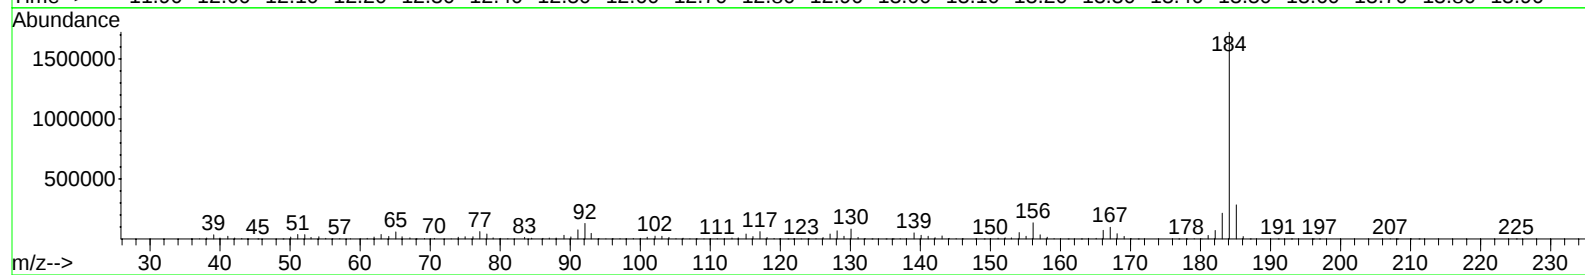


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080818\
Data File : BF108005.D
Acq On : 8 Aug 2018 8:33
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 17:13:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

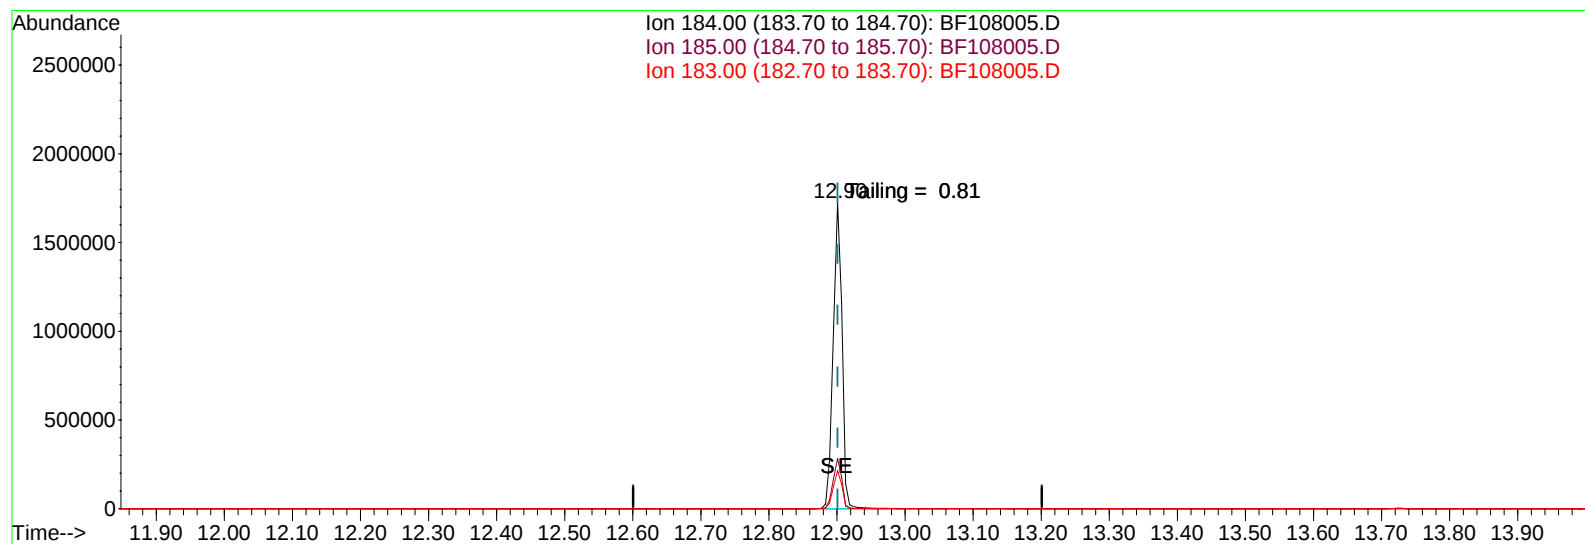

(76) Benzidine




12.901min (+0.000) 50206.38ng

response 1562569

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.49
183.00	11.60	12.47
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080818\
Data File : BF108005.D
Acq On : 8 Aug 2018 8:33
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 17:13:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

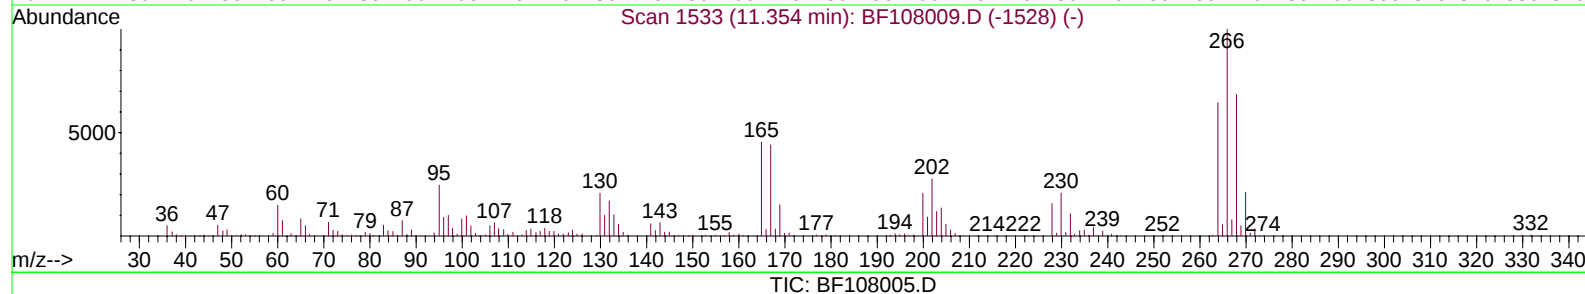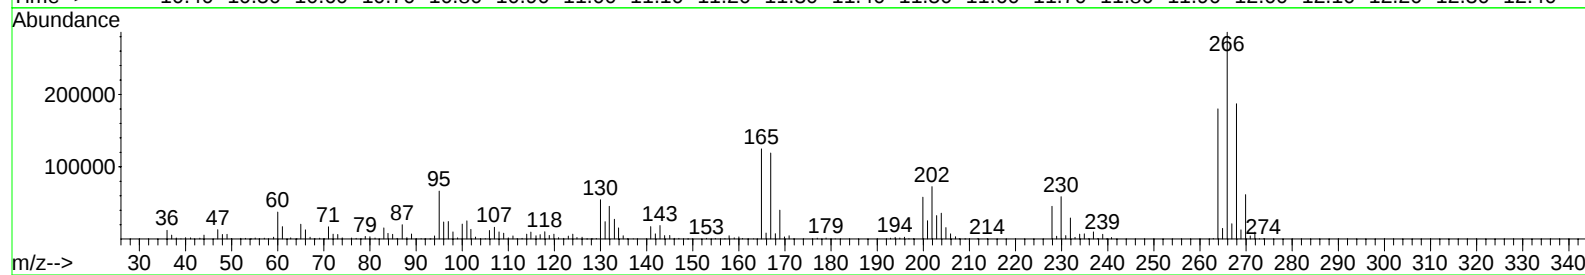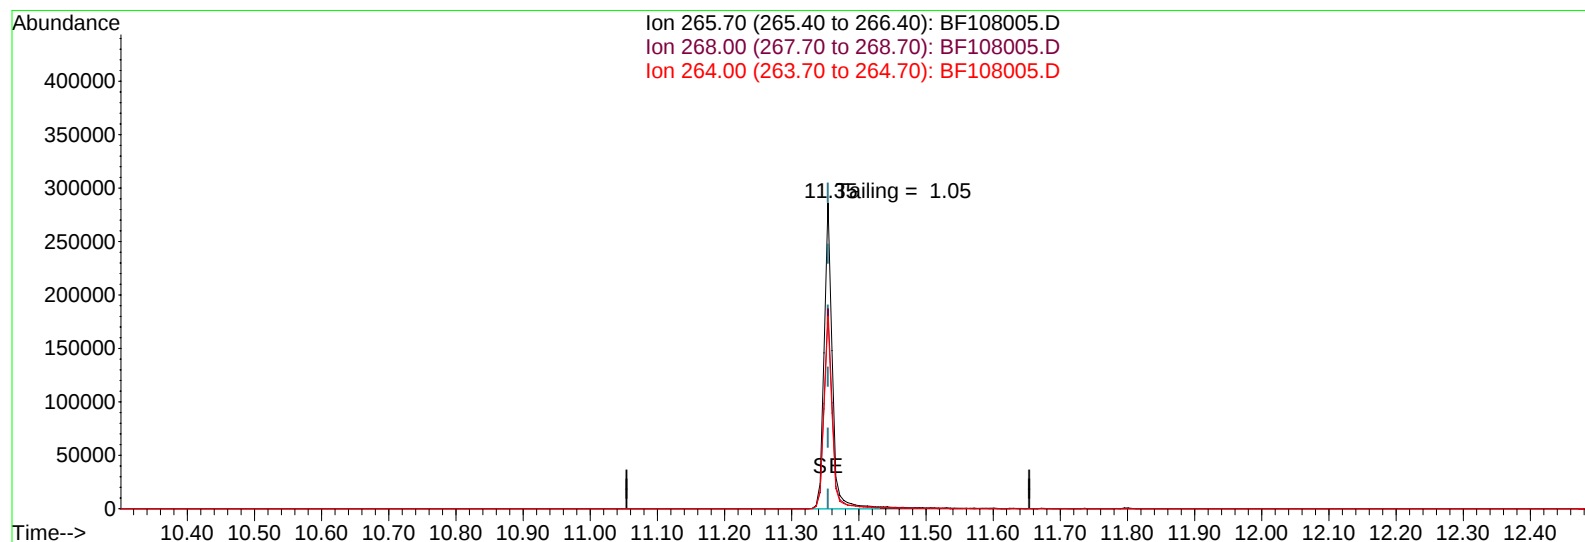

(69) Pentachlorophenol (C)

11.354min (+0.000) 65428.98ng

response 245646

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.44
264.00	61.90	62.95
0.00	0.00	0.00