

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080818\
 Data File : BF108028.D
 Acq On : 8 Aug 2018 19:12
 Operator : JU/SJ
 Sample : J3762-07
 Misc : LOD 2 PPM
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2018

Quant Time: Aug 09 07:23:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 12:24:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.01	152	275156	20.00	ng	0.00
21) Naphthalene-d8	8.30	136	1091268	20.00	ng	0.00
38) Acenaphthene-d10	10.06	164	597002	20.00	ng	0.00
63) Phenanthrene-d10	11.55	188	1234980	20.00	ng	0.00
75) Chrysene-d12	14.21	240	1120053	20.00	ng	-0.01
86) Perylene-d12	15.77	264	986885	20.00	ng	-0.01

System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	1940212	127.66	ng	0.00
7) Phenol-d6	6.63	99	2581007	127.80	ng	0.00
23) Nitrobenzene-d5	7.58	82	1706956	87.28	ng	0.00
41) 2,4,6-Tribromophenol	10.85	330	832774	139.85	ng	0.00
44) 2-Fluorobiphenyl	9.38	172	3055256	82.16	ng	0.00
78) Terphenyl-d14	0.00	244	0d	0.00	ng	


Target Compounds				Qvalue		
17) 2-Methylphenol	7.24	107	34533	2.353	ng	93
19) n-Nitroso-di-n-propylamine	7.41	70	29752	2.178	ng	# 86
20) 3+4-Methylphenols	7.40	107	41656	2.214	ng	94
22) Acetophenone	7.41	105	59772	2.342	ng	93
25) Isophorone	7.82	82	78607	2.109	ng	# 93
26) 2-Nitrophenol	7.91	139	11607	1.554	ng	97
27) 2,4-Dimethylphenol	7.93	122	41704	2.521	ng	97
28) bis(2-Chloroethoxy)methane	8.03	93	48609	2.234	ng	# 96
29) 2,4-Dichlorophenol	8.14	162	29317	1.926	ng	94
30) 1,2,4-Trichlorobenzene	8.23	180	39063	2.327	ng	93
36) 4-Chloro-3-methylphenol	8.82	107	32882	2.002	ng	99
42) 2,4,6-Trichlorophenol	9.28	196	19161	1.684	ng	99
43) 2,4,5-Trichlorophenol	9.31	196	23831	1.903	ng	95
56) 2,4-Dinitrotoluene	10.23	165	20161	1.800	ng	# 85
60) 4-Chlorophenyl-phenylether	10.60	204	47287	2.349	ng	89
61) 4-Nitroaniline	10.61	138	17248	1.833	ng	84
76) Benzidine	12.89	184	20492	0.490	ng	# 93
81) 3,3'-Dichlorobenzidine	14.15	252	25349	1.100	ng	# 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080818\
Data File : BF108028.D
Acq On : 8 Aug 2018 19:12
Operator : JU/SJ
Sample : J3762-07
Misc : LOD 2 PPM
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

Quant Time: Aug 09 07:23:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

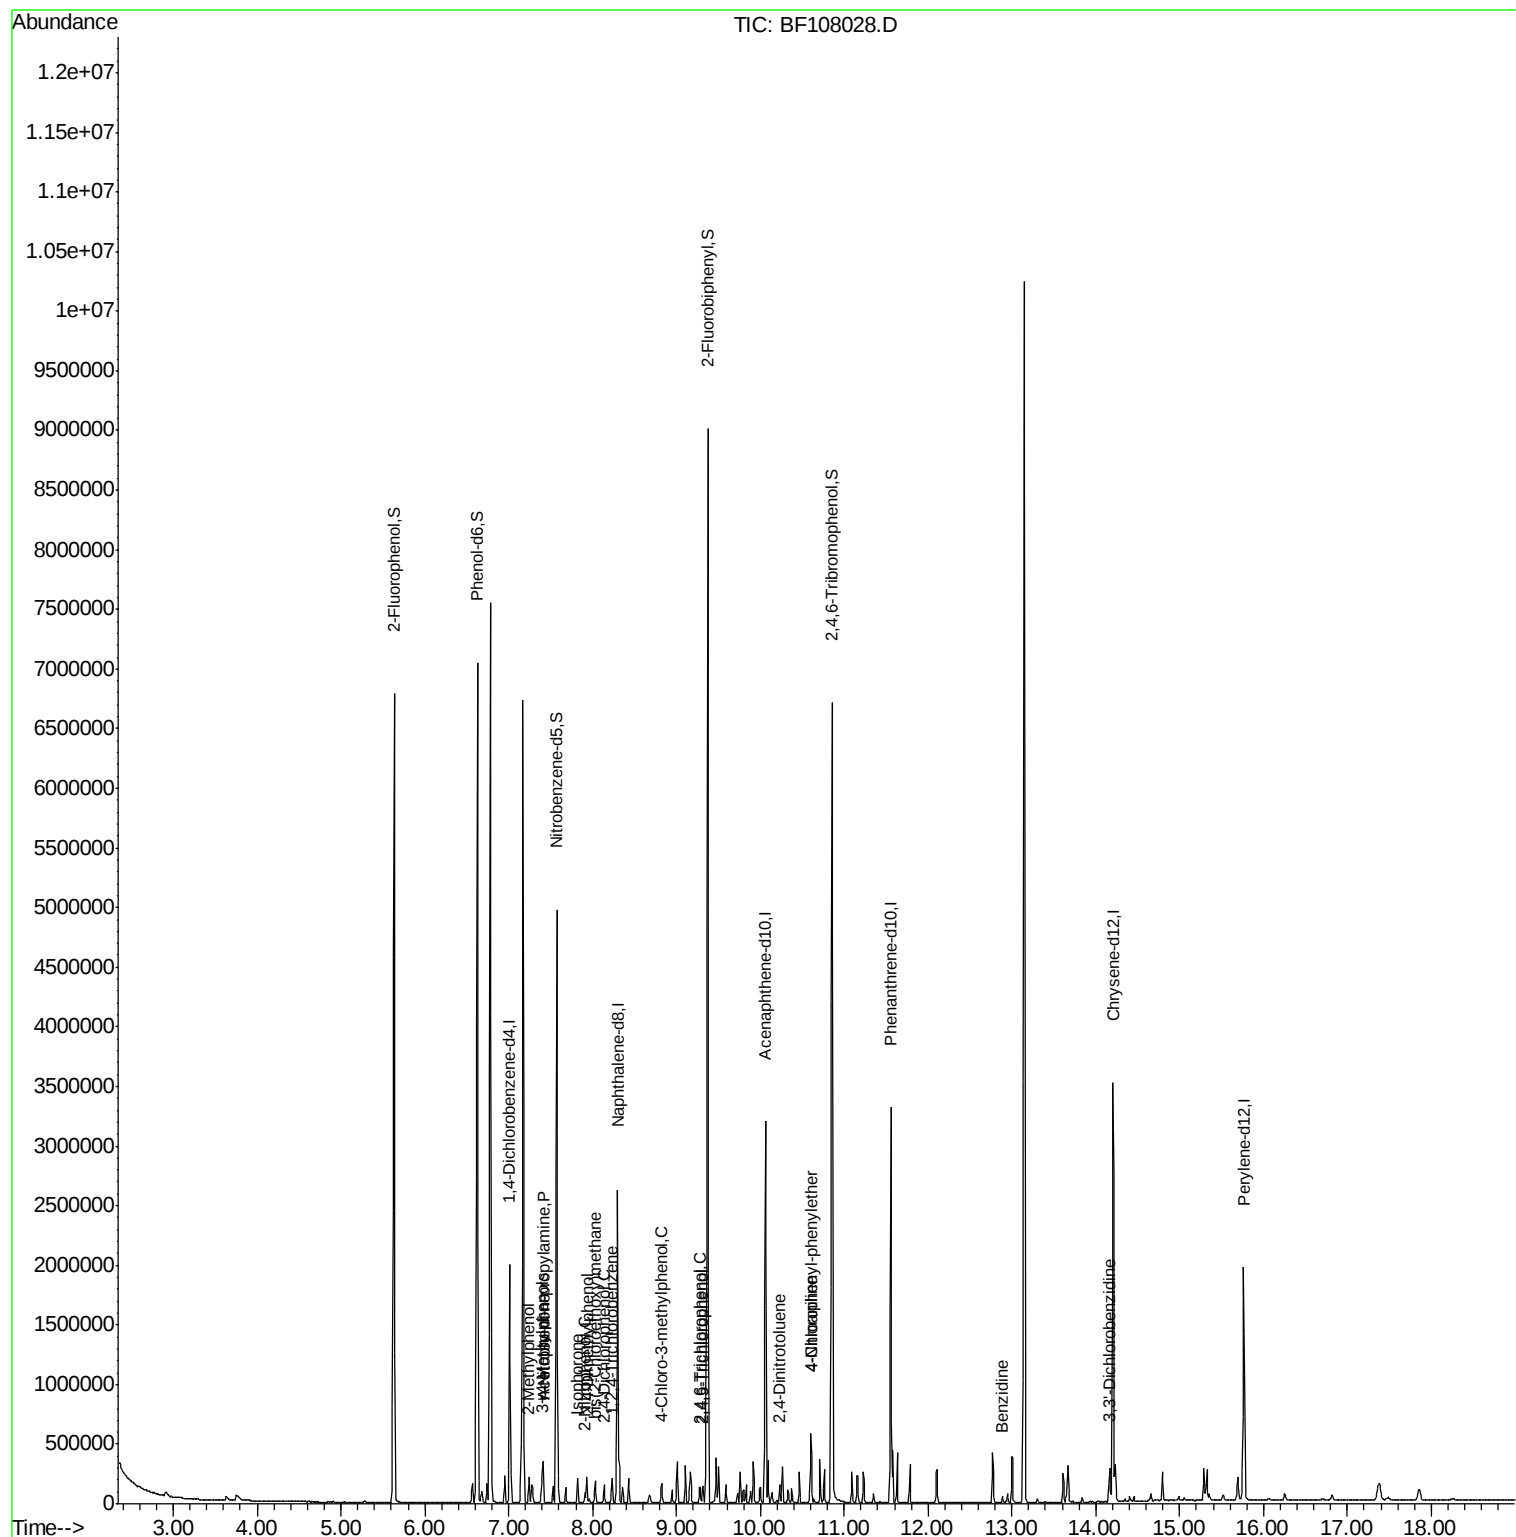




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.01 min Scan# 795
Delta R.T. 0.00 min
Lab File: BF108028.D
Acq: 8 Aug 2018 19:12

Instrument :
BNA_F
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

Tot Ion:152 Resp: 275156
Ion Ratio Lower Upper
152 100
150 155.4 124.6 186.8
115 61.7 50.1 75.1

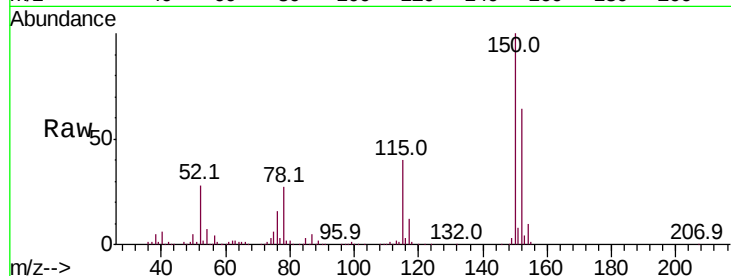


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

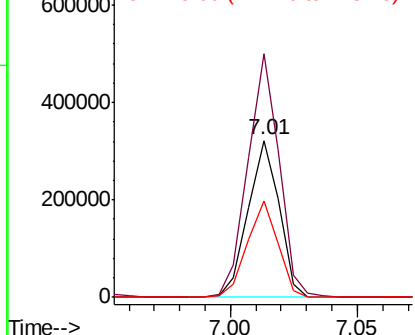



#5


2-Fluorophenol
Concen: 127.661 ng
RT: 5.64 min Scan# 561
Delta R.T. 0.01 min
Lab File: BF108028.D
Acq: 8 Aug 2018 19:12

Tgt Ion:112 Resp: 1940212
Ion Ratio Lower Upper
112 100
64 69.9 47.9 71.9
63 38.1 23.7 35.5#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

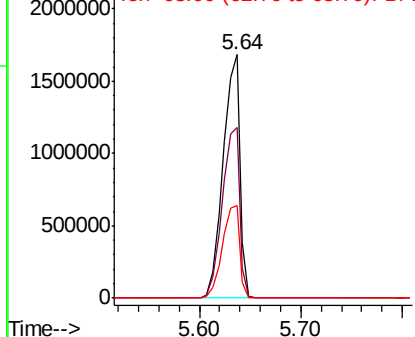

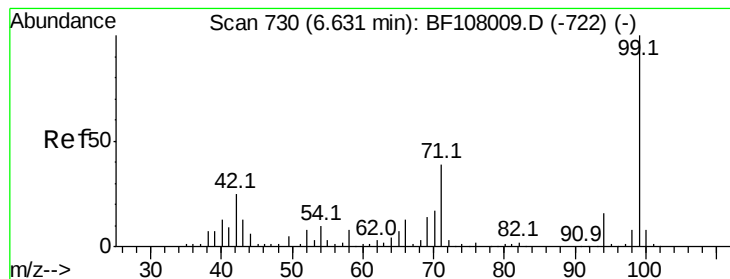

#7

Phenol-d6

Concen: 127.796 ng

RT: 6.63 min Scan# 730

Delta R.T. 0.00 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12

Instrument :

BNA_F

ClientSampleId :

LOD-MDL-WATER-01-QT3-2018


Tot Ion: 99 Resp: 2581007

Ion Ratio Lower Upper




99 100

42 26.8 14.5 21.7#

71 41.0 25.4 38.0#

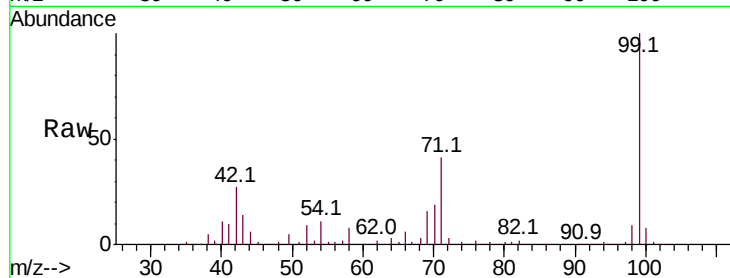

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

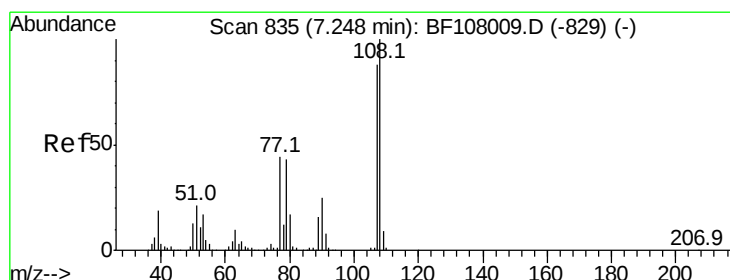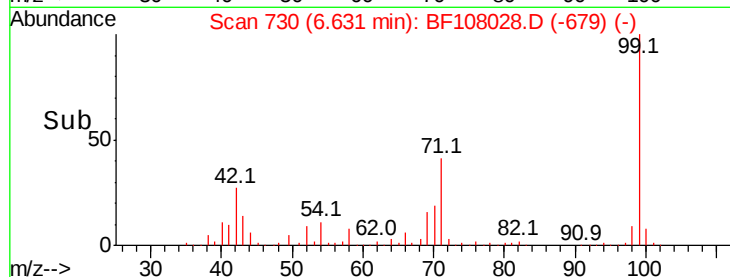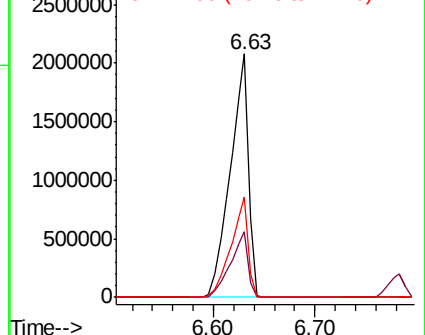

#17

2-Methylphenol

Concen: 2.353 ng

RT: 7.24 min Scan# 834

Delta R.T. -0.01 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12

Tgt Ion:107 Resp: 34533


Ion Ratio Lower Upper

107 100



108 105.1 91.7 137.5


77 46.7 33.8 50.8

79 45.0 33.8 50.8

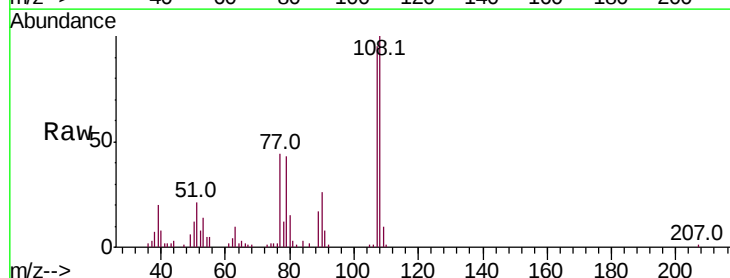

Abundance Ion 107.00 (106.70 to 107.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 77.00 (76.70 to 77.70): BF1
Ion 79.00 (78.70 to 79.70): BF1



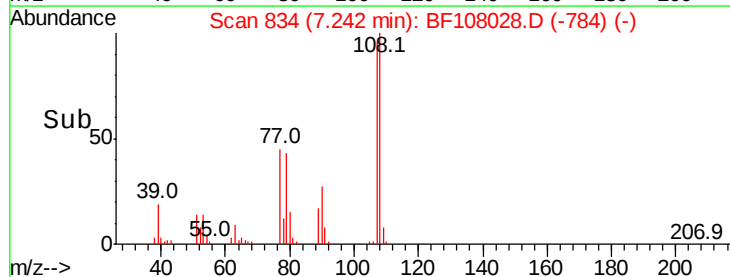
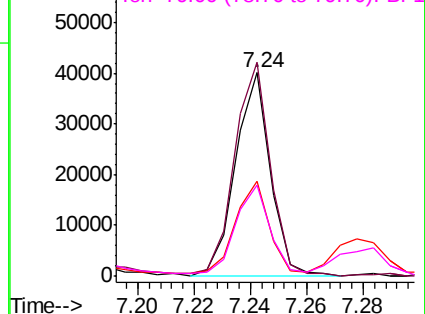


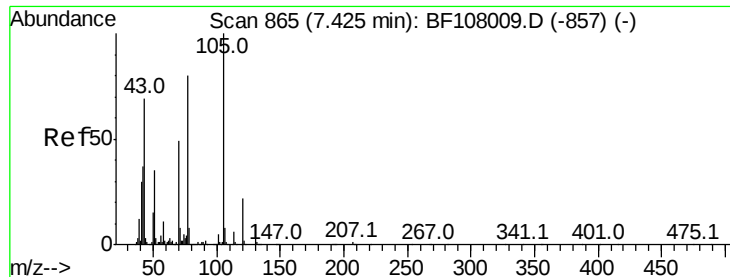

#19
n-Nitroso-di-n-propylamine
Concen: 2.178 ng
RT: 7.41 min Scan# 862
Delta R.T. -0.02 min
Lab File: BF108028.D
Acq: 8 Aug 2018 19:12




Instrument :
BNA_F
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018


Tot Ion: 70 Resp: 29752
Ion Ratio Lower Upper
70 100
42 75.3 47.5 71.3#
101 9.5 7.4 11.2
130 20.4 16.6 25.0

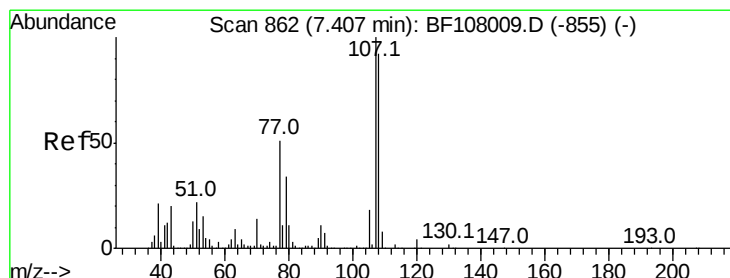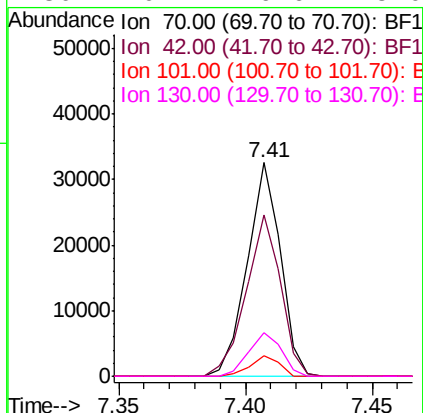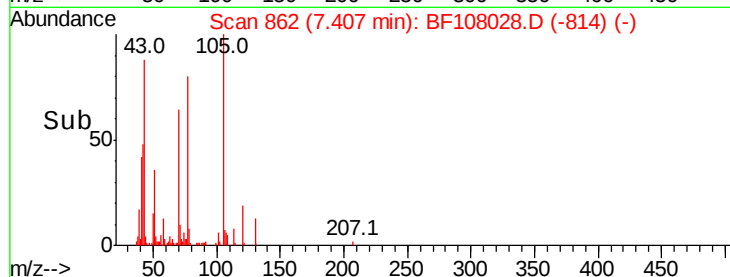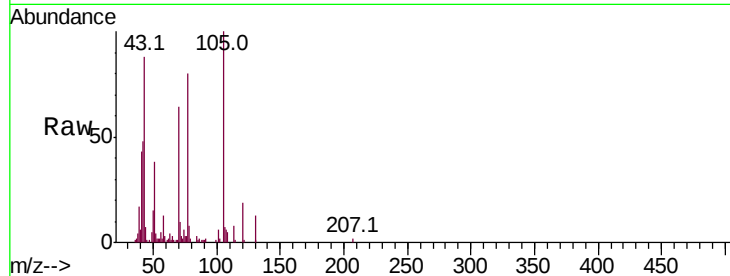

#20
3+4-Methylphenols
Concen: 2.214 ng
RT: 7.40 min Scan# 860
Delta R.T. -0.01 min
Lab File: BF108028.D
Acq: 8 Aug 2018 19:12

Tgt Ion:107 Resp: 41656
Ion Ratio Lower Upper
107 100
108 88.6 68.2 108.2
77 36.3 26.7 66.7
79 29.4 6.3 46.3

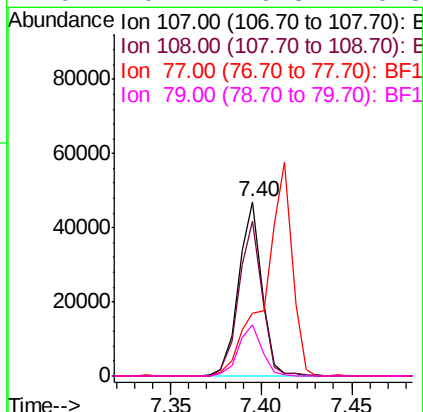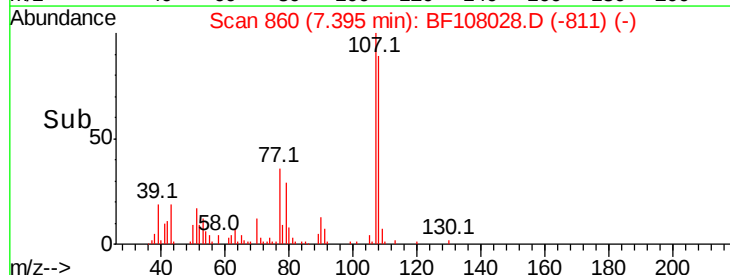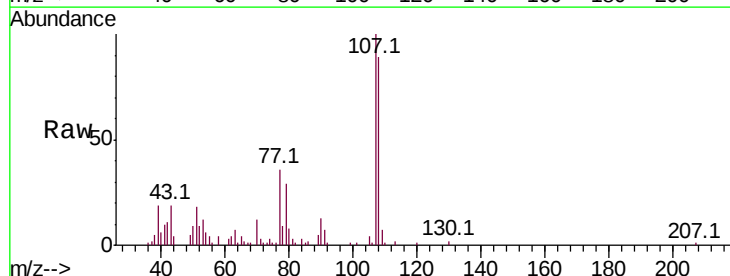



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.30 min Scan# 1013

Delta R.T. -0.01 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12

Instrument :

BNA_F


ClientSampleId :

LOD-MDL-WATER-01-QT3-2018

Tot Ion:136 Resp: 1091268

Ion Ratio Lower Upper

136	100		
137	11.4	8.9	13.3
54	11.2	6.6	9.8#
68	6.4	5.0	7.4



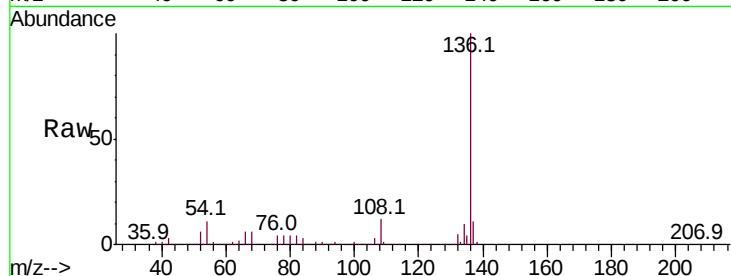


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

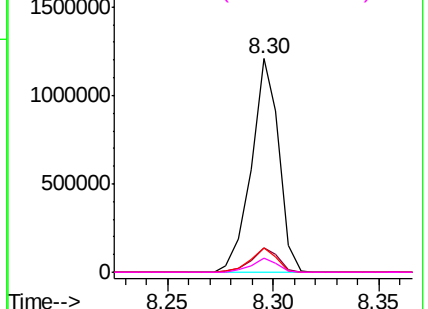

#22

Acetophenone

Concen: 2.342 ng

RT: 7.41 min Scan# 863

Delta R.T. -0.01 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12

Tgt Ion:105 Resp: 59772

Ion Ratio Lower Upper




105	100		
71	5.1	4.4	6.6
51	32.2	22.3	33.5
120	24.0	16.9	25.3


Abundance Ion 105.00 (104.70 to 105.70): E

Ion 71.00 (70.70 to 71.70): BF1

Ion 51.00 (50.70 to 51.70): BF1

Ion 120.00 (119.70 to 120.70): E

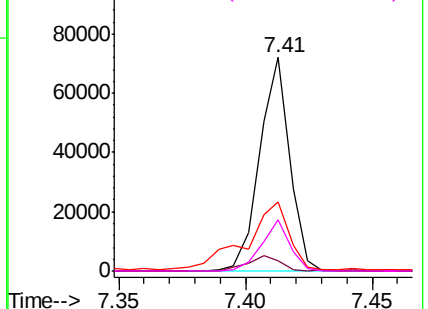







#23
 Nitrobenzene-d5
 Concen: 87.284 ng
 RT: 7.58 min Scan# 891
 Delta R.T. 0.00 min
 Lab File: BF108028.D
 Acq: 8 Aug 2018 19:12

Instrument :
 BNA_F
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2018

Tot Ion: 82 Resp: 1706956
 Ion Ratio Lower Upper
 82 100
 128 43.0 36.1 54.1
 54 62.2 41.4 62.2#

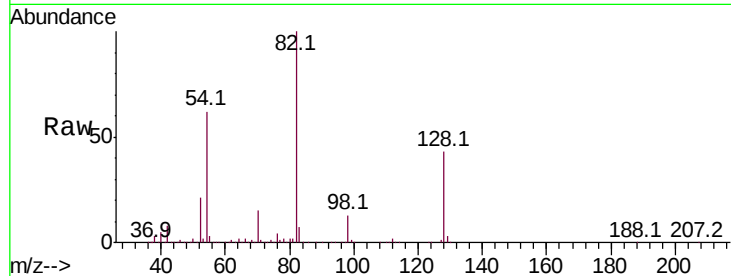


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1


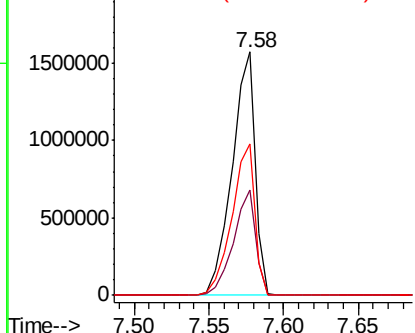



#25
 Isophorone
 Concen: 2.109 ng
 RT: 7.82 min Scan# 932
 Delta R.T. -0.02 min
 Lab File: BF108028.D
 Acq: 8 Aug 2018 19:12

Tgt Ion: 82 Resp: 78607
 Ion Ratio Lower Upper
 82 100
 95 7.0 5.2 7.8
 138 14.7 14.9 22.3#

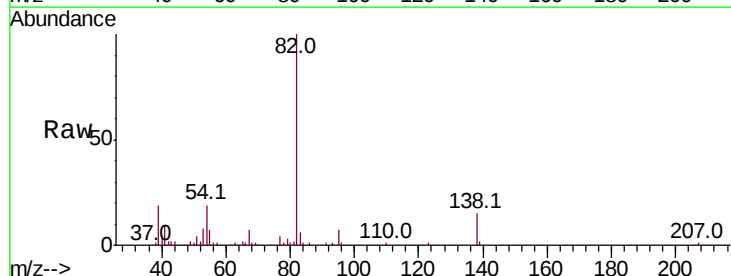

Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 95.00 (94.70 to 95.70): BF1
 Ion 138.00 (137.70 to 138.70): BF1

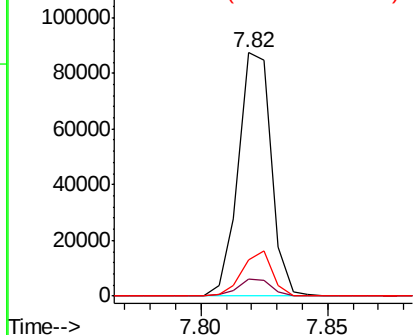



#26

2-Nitrophenol

Concen: 1.554 ng

RT: 7.91 min Scan# 947

Delta R.T. -0.01 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12

Instrument :

BNA_F

ClientSampleId :

LOD-MDL-WATER-01-QT3-2018


Tot Ion:139 Resp: 11607

Ion Ratio Lower Upper

139 100

109 31.9 22.7 34.1




65 51.5 40.5 60.7

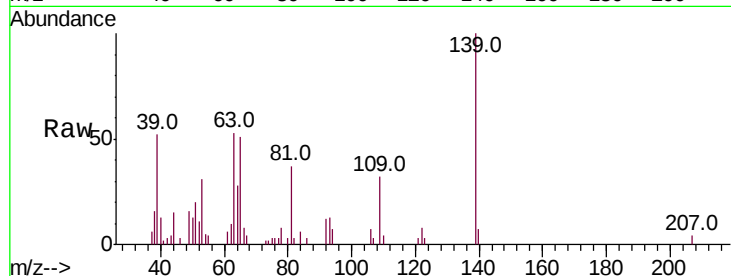

Abundance Ion 139.00 (138.70 to 139.70): E

Ion 109.00 (108.70 to 109.70): E

Ion 65.00 (64.70 to 65.70): BF1

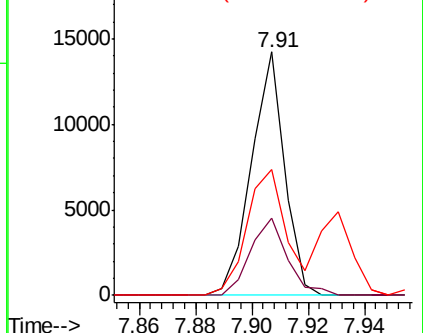

#27

2,4-Dimethylphenol

Concen: 2.521 ng

RT: 7.93 min Scan# 951

Delta R.T. -0.01 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12


Tgt Ion:122 Resp: 41704

Ion Ratio Lower Upper

122 100

107 118.1 91.2 136.8



121 60.3 47.2 70.8




Abundance Ion 122.00 (121.70 to 122.70): E

Ion 107.00 (106.70 to 107.70): E

Ion 121.00 (120.70 to 121.70): E

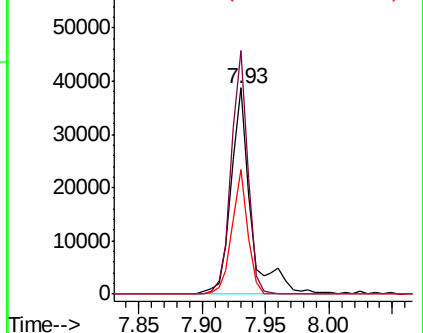



#28

bis(2-Chloroethoxy)methane

Concen: 2.234 ng

RT: 8.03 min Scan# 968

Delta R.T. -0.01 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12

Instrument :

BNA_F

ClientSampleId :

LOD-MDL-WATER-01-QT3-2018





Tot Ion: 93 Resp: 48609

Ion Ratio Lower Upper

93 100

95 31.2 26.3 39.5

123 9.6 9.8 14.6#

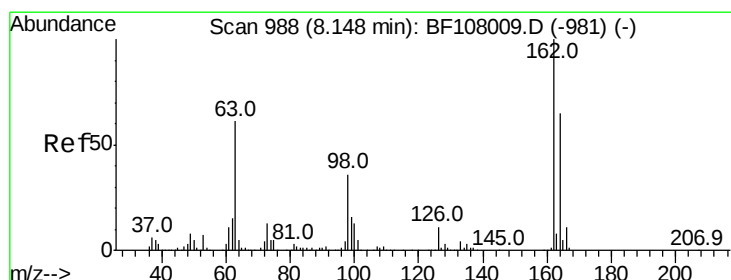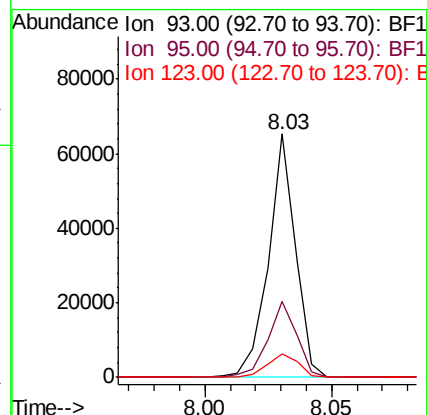

#29

2,4-Dichlorophenol

Concen: 1.926 ng

RT: 8.14 min Scan# 987

Delta R.T. -0.01 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12




Tgt Ion:162 Resp: 29317


Ion Ratio Lower Upper

162 100

164 69.2 42.7 82.7

98 36.6 18.1 58.1

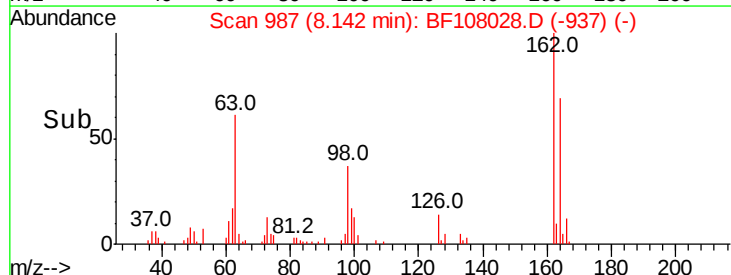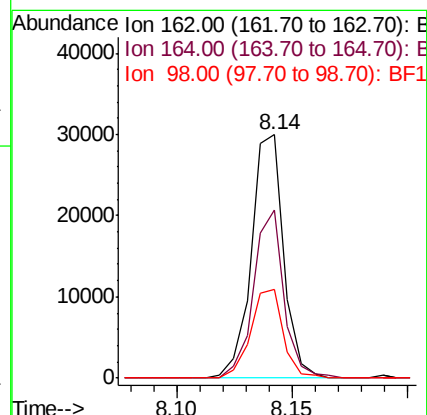







#30
 1,2,4-Trichlorobenzene
 Concen: 2.327 ng
 RT: 8.23 min Scan# 1002
 Delta R.T. -0.01 min
 Lab File: BF108028.D
 Acq: 8 Aug 2018 19:12

Instrument :
 BNA_F
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2018

Tot Ion:180 Resp: 39063
 Ion Ratio Lower Upper
 180 100
 182 90.1 76.8 115.2
 145 28.6 26.5 39.7

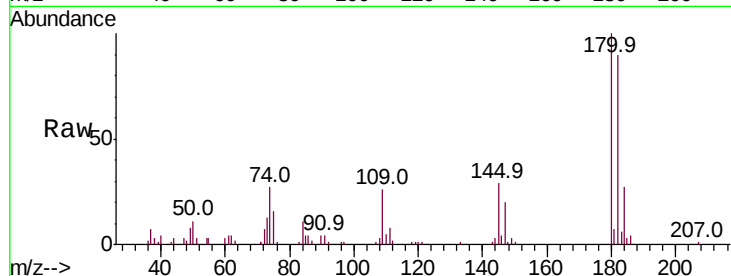


Abundance Ion 180.00 (179.70 to 180.70): E
 Ion 182.00 (181.70 to 182.70): E
 Ion 145.00 (144.70 to 145.70): E


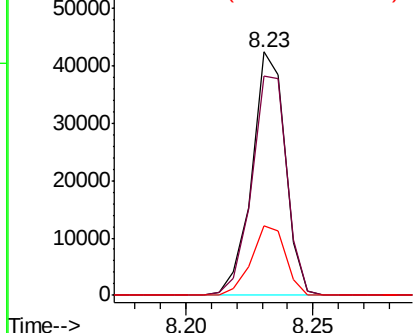



#36
 4-Chloro-3-methylphenol
 Concen: 2.002 ng
 RT: 8.82 min Scan# 1103
 Delta R.T. -0.01 min
 Lab File: BF108028.D
 Acq: 8 Aug 2018 19:12

Tgt Ion:107 Resp: 32882
 Ion Ratio Lower Upper
 107 100
 144 24.3 20.5 30.7
 142 76.5 62.0 93.0



Abundance Ion 107.00 (106.70 to 107.70): E
 Ion 144.00 (143.70 to 144.70): E
 Ion 142.00 (141.70 to 142.70): E

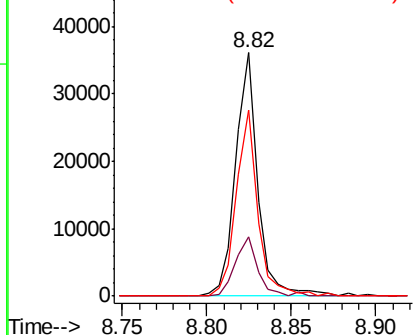







#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.06 min Scan# 1313
 Delta R.T. -0.01 min
 Lab File: BF108028.D
 Acq: 8 Aug 2018 19:12

Instrument :
 BNA_F
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2018

Tot Ion:164 Resp: 597002
 Ion Ratio Lower Upper
 164 100
 162 102.7 86.1 129.1
 160 46.7 38.3 57.5




Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E


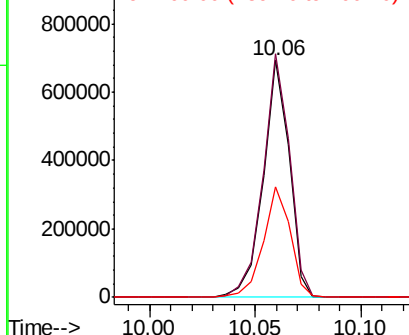



#41
 2,4,6-Tribromophenol
 Concen: 139.846 ng
 RT: 10.85 min Scan# 1448
 Delta R.T. -0.01 min
 Lab File: BF108028.D
 Acq: 8 Aug 2018 19:12

Tgt Ion:330 Resp: 832774
 Ion Ratio Lower Upper
 330 100
 332 96.4 77.0 115.6
 141 34.4 29.9 44.9



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

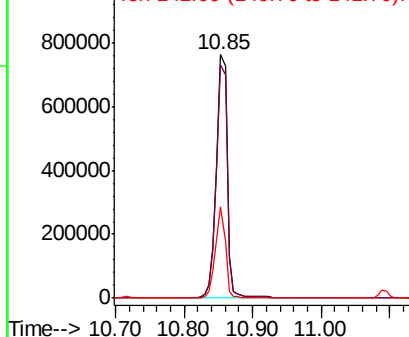







#42
 2,4,6-Trichlorophenol
 Concen: 1.684 ng
 RT: 9.28 min Scan# 1180
 Delta R.T. -0.01 min
 Lab File: BF108028.D
 Acq: 8 Aug 2018 19:12

Instrument :
 BNA_F
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2018

Tot Ion:196 Resp: 19161
 Ion Ratio Lower Upper
 196 100
 198 95.6 75.7 113.5
 200 29.6 24.5 36.7

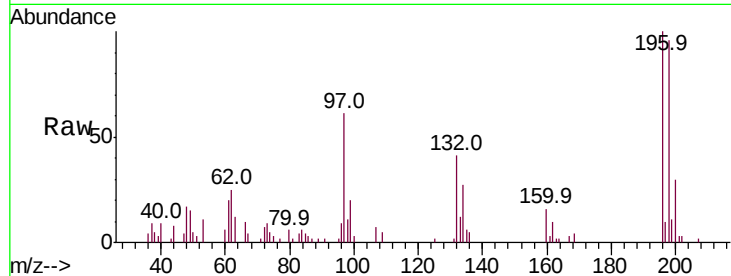




Abundance Ion 196.00 (195.70 to 196.70): E
 Ion 198.00 (197.70 to 198.70): E
 Ion 200.00 (199.70 to 200.70): E

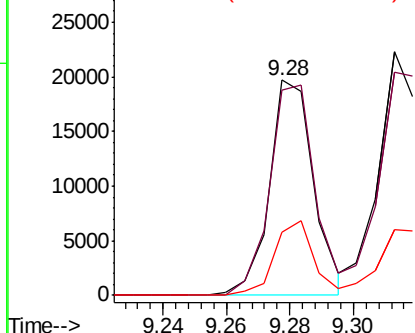


#43
 2,4,5-Trichlorophenol
 Concen: 1.903 ng
 RT: 9.31 min Scan# 1186
 Delta R.T. -0.01 min
 Lab File: BF108028.D
 Acq: 8 Aug 2018 19:12

Tgt Ion:196 Resp: 23831
 Ion Ratio Lower Upper
 196 100
 198 91.4 74.6 112.0
 97 47.4 42.9 64.3
 132 30.0 26.3 39.5

Abundance Ion 196.00 (195.70 to 196.70): E
 Ion 198.00 (197.70 to 198.70): E
 Ion 97.00 (96.70 to 97.70): BF1
 Ion 132.00 (131.70 to 132.70): E

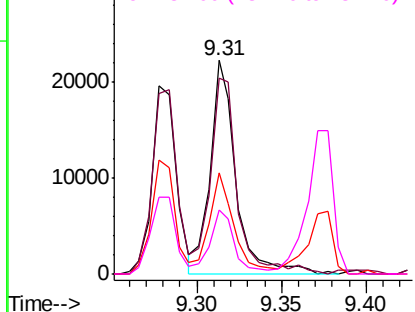







#44
2-Fluorobiphenyl
Concen: 82.163 ng
RT: 9.38 min Scan# 1197
Delta R.T. 0.00 min
Lab File: BF108028.D
Acq: 8 Aug 2018 19:12

Instrument :
BNA_F
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

Tot Ion:172 Resp: 3055256
Ion Ratio Lower Upper
172 100
171 41.8 29.7 44.5
170 28.2 19.6 29.4




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


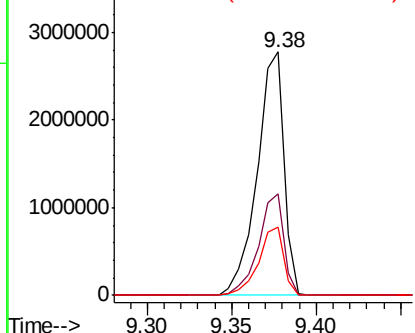



#56
2,4-Dinitrotoluene
Concen: 1.800 ng
RT: 10.23 min Scan# 1342
Delta R.T. -0.02 min
Lab File: BF108028.D
Acq: 8 Aug 2018 19:12

Tgt Ion:165 Resp: 20161
Ion Ratio Lower Upper
165 100
63 53.6 36.4 54.6
89 86.9 57.8 86.6#
182 2.4 1.6 2.4



Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1
Ion 182.00 (181.70 to 182.70): E

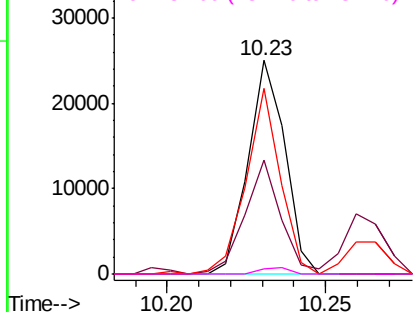







#60
4-Chlorophenyl-phenylether
Concen: 2.349 ng
RT: 10.60 min Scan# 1405
Delta R.T. -0.01 min
Lab File: BF108028.D
Acq: 8 Aug 2018 19:12

Instrument :
BNA_F
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

Tot Ion:204 Resp: 47287
Ion Ratio Lower Upper
204 100
206 34.3 26.5 39.7
141 56.4 54.6 81.8

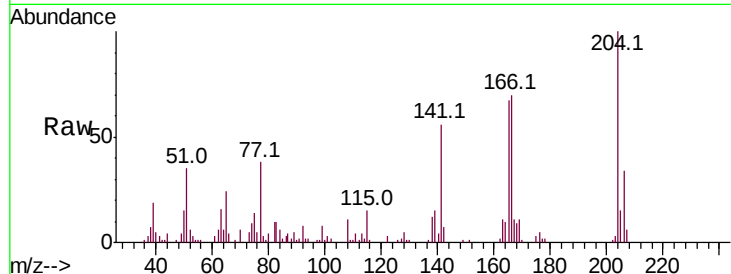


Abundance Ion 204.00 (203.70 to 204.70): E
Ion 206.00 (205.70 to 206.70): E
Ion 141.00 (140.70 to 141.70): E

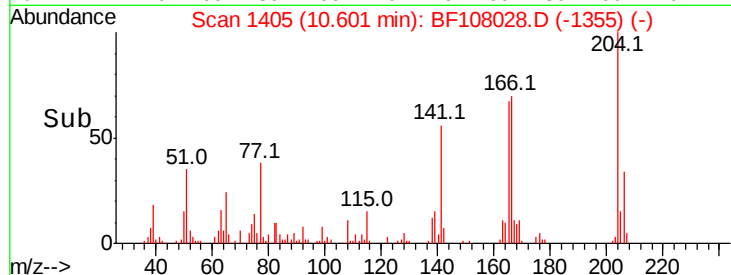
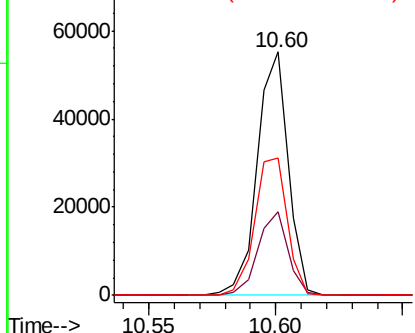



#61
4-Nitroaniline
Concen: 1.833 ng
RT: 10.61 min Scan# 1406
Delta R.T. -0.03 min
Lab File: BF108028.D
Acq: 8 Aug 2018 19:12

Tgt Ion:138 Resp: 17248
Ion Ratio Lower Upper
138 100
92 58.4 30.2 70.2
108 88.2 52.5 92.5

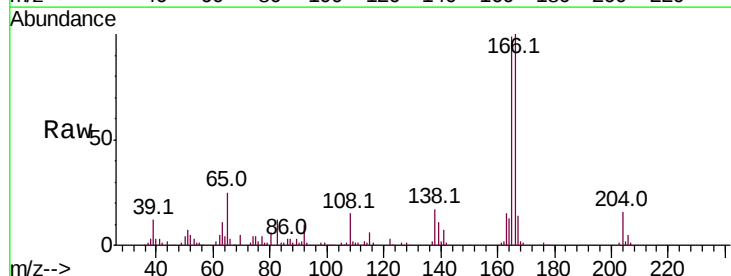

Abundance Ion 138.00 (137.70 to 138.70): E
Ion 92.00 (91.70 to 92.70): BF1
Ion 108.00 (107.70 to 108.70): E

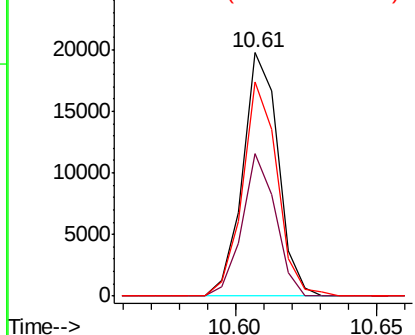



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.55 min Scan# 1567

Delta R.T. -0.01 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12

Instrument :

BNA_F

ClientSampleId :

LOD-MDL-WATER-01-QT3-2018


Tot Ion:188 Resp: 1234980

Ion Ratio Lower Upper

188 100

94 9.7 8.5 12.7




80 11.1 9.2 13.8



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

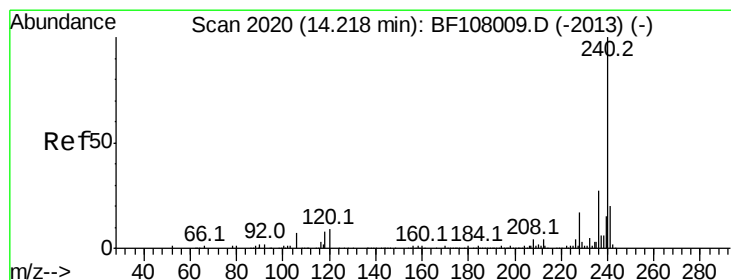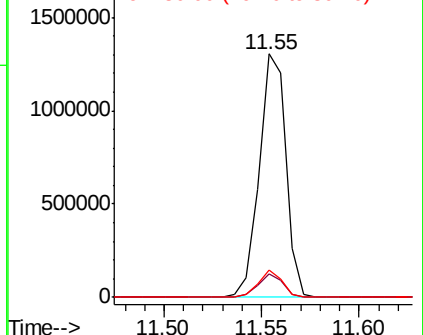

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.21 min Scan# 2018

Delta R.T. -0.01 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12


Tgt Ion:240 Resp: 1120053

Ion Ratio Lower Upper

240 100

120 11.4 9.5 14.3



236 27.2 20.7 31.1




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

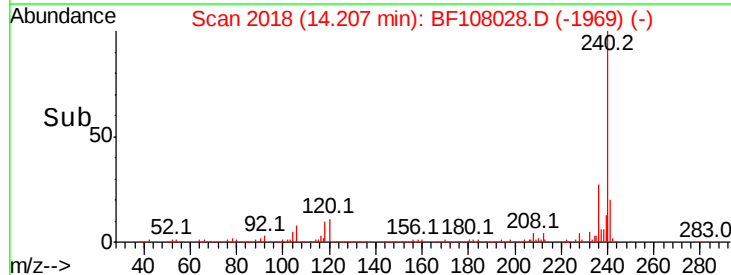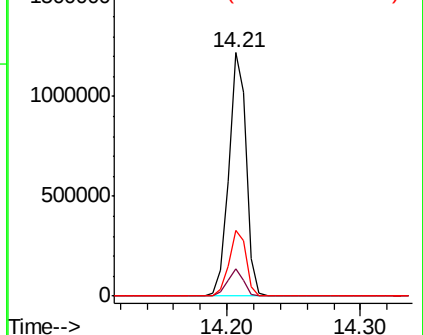



#76

Benzidine

Concen: 0.490 ng

RT: 12.89 min Scan# 1794

Delta R.T. -0.01 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12

Instrument :

BNA_F

ClientSampleId :

LOD-MDL-WATER-01-QT3-2018


Tot Ion:184 Resp: 20492

Ion Ratio Lower Upper

184 100

185 19.4 12.6 18.8#




183 13.7 9.3 13.9



Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

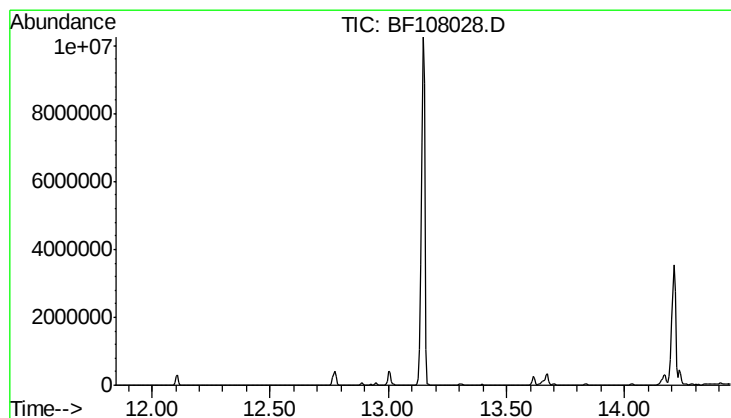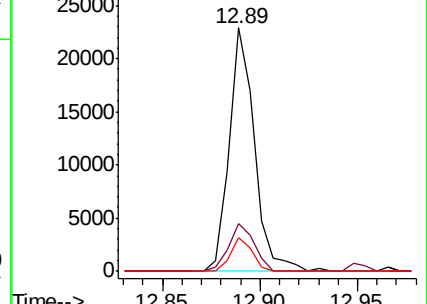

#78

Terphenyl-d14

Concen: 0.000 ng

Expected RT: 13.15 min

Lab File: BF108028.D

Acq: 8 Aug 2018 19:12

Tgt Ion: 244


Sig Exp Ratio

244 100

212 6.7

122 13.7









#81
 3,3'-Dichlorobenzidine
 Concen: 1.100 ng
 RT: 14.15 min Scan# 2009
 Delta R.T. -0.01 min
 Lab File: BF108028.D
 Acq: 8 Aug 2018 19:12

Instrument :
 BNA_F
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2018

Tot Ion	Ratio	Lower	Upper
252	100		
254	59.4	50.4	75.6
126	11.1	11.3	16.9

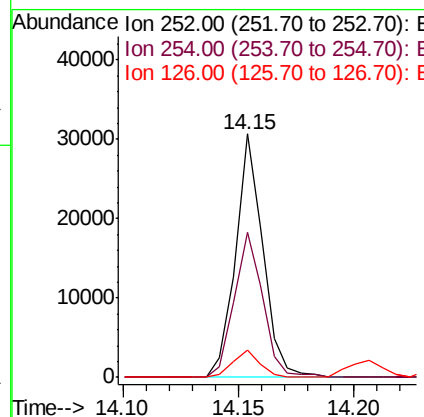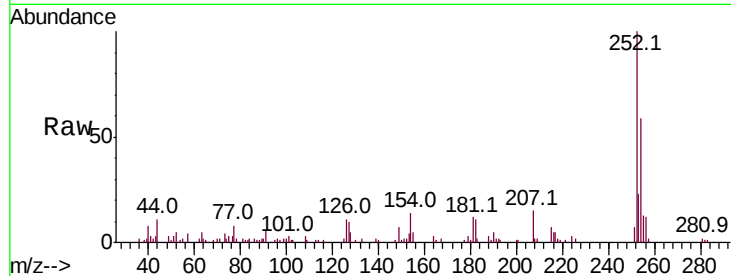

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.77 min Scan# 2283
 Delta R.T. -0.01 min
 Lab File: BF108028.D
 Acq: 8 Aug 2018 19:12

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.2	28.8
265	21.8	17.5	26.3

