


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080818\
 Data File : BF108005.D
 Acq On : 8 Aug 2018 8:33
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 12:24:24 2018

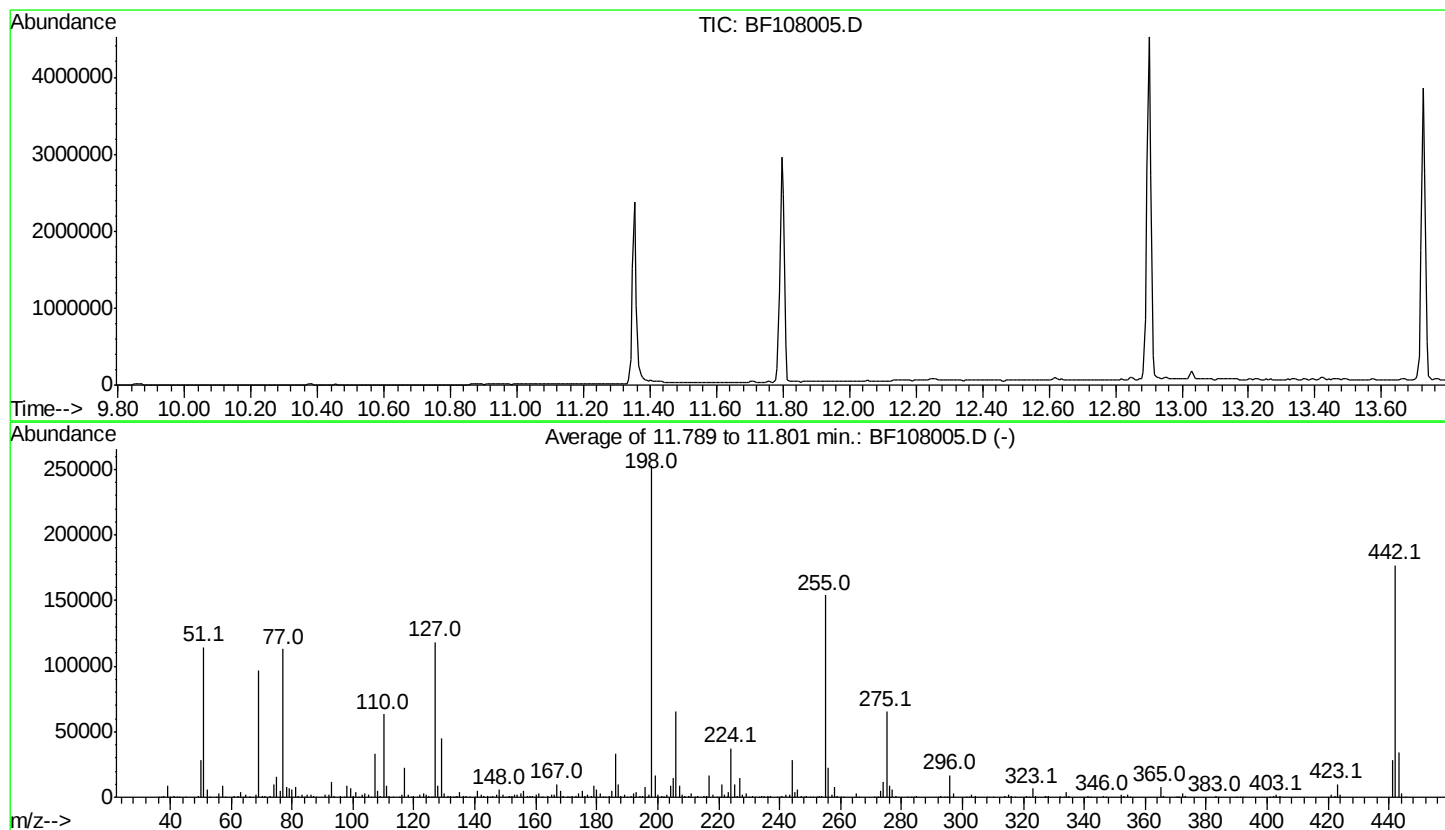

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	114440	PASS
68	69	0.00	2	1.9	1863	PASS
69	198	0.00	100	38.1	96273	PASS
70	69	0.00	2	0.7	633	PASS
127	198	10	80	46.9	118437	PASS
197	198	0.00	2	0.6	1553	PASS
198	198	100	100	100.0	252714	PASS
199	198	5	9	6.6	16599	PASS
275	198	10	60	25.8	65120	PASS
365	198	1	100	3.1	7836	PASS
441	198	0.01	100	11.3	28612	PASS
442	198	50	100	69.9	176698	PASS
443	442	15	24	19.2	33975	PASS