


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080819\
 Data File : BF116059.D
 Acq On : 8 Aug 2019 10:20
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

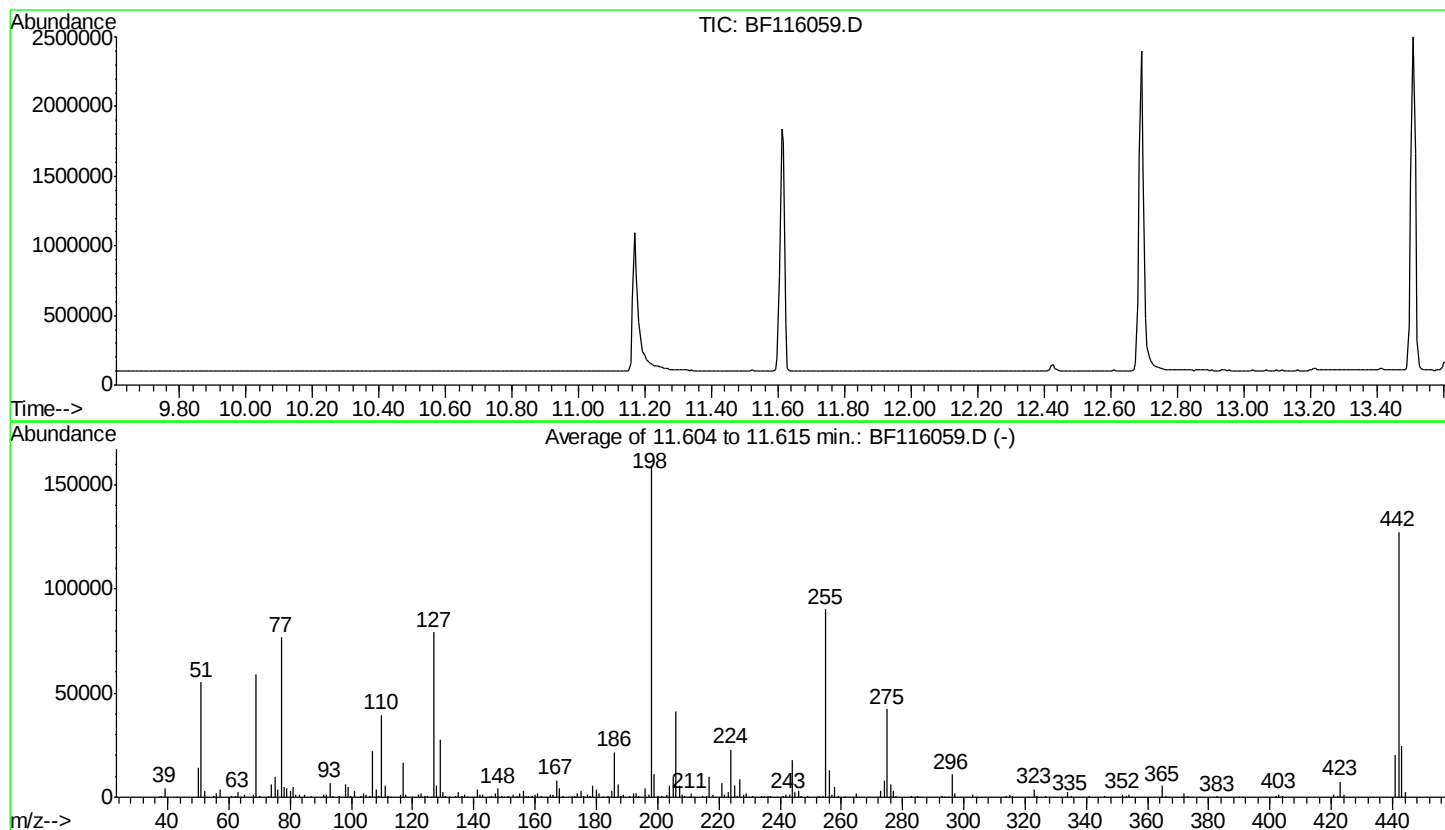

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	55211	PASS
68	69	0.00	2	1.6	957	PASS
69	198	0.00	100	37.0	58840	PASS
70	69	0.00	2	0.9	513	PASS
127	198	10	80	49.8	79181	PASS
197	198	0.00	2	0.7	1048	PASS
198	198	100	100	100.0	159112	PASS
199	198	5	9	7.0	11115	PASS
275	198	10	60	26.6	42312	PASS
365	198	1	100	3.3	5279	PASS
441	198	0.01	100	12.8	20310	PASS
442	198	50	100	80.1	127461	PASS
443	442	15	24	19.4	24747	PASS