


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080819\
 Data File : BF116074.D
 Acq On : 8 Aug 2019 18:02
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

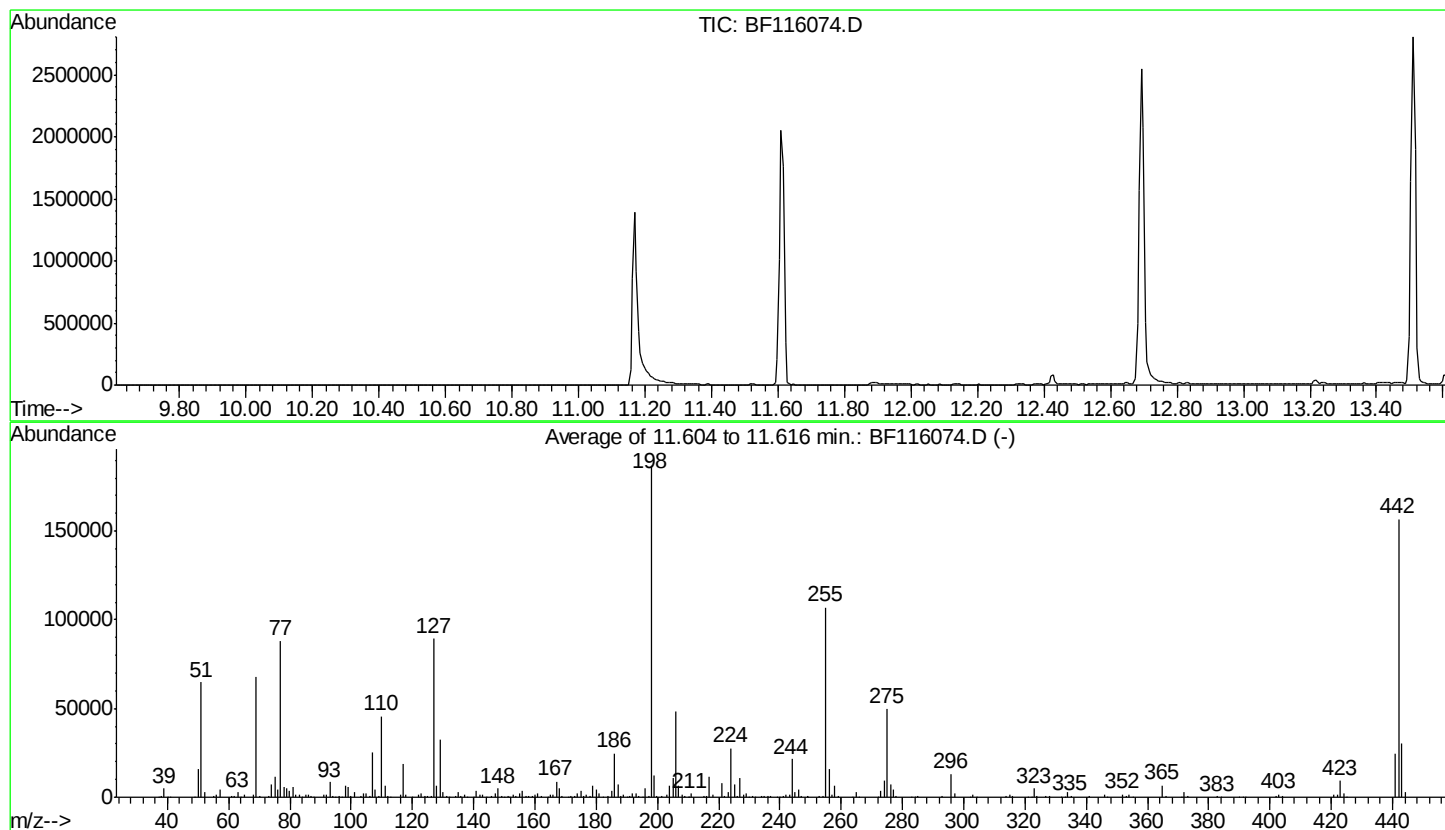

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	64757	PASS
68	69	0.00	2	1.7	1163	PASS
69	198	0.00	100	36.3	67890	PASS
70	69	0.00	2	0.7	443	PASS
127	198	10	80	47.7	89157	PASS
197	198	0.00	2	0.6	1057	PASS
198	198	100	100	100.0	186866	PASS
199	198	5	9	6.7	12595	PASS
275	198	10	60	26.7	49848	PASS
365	198	1	100	3.5	6631	PASS
441	198	0.01	100	13.0	24321	PASS
442	198	50	100	83.9	156810	PASS
443	442	15	24	19.5	30595	PASS