


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080823\
Data File : BF134661.D
Acq On : 08 Aug 2023 08:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 04 09:29:15 2023

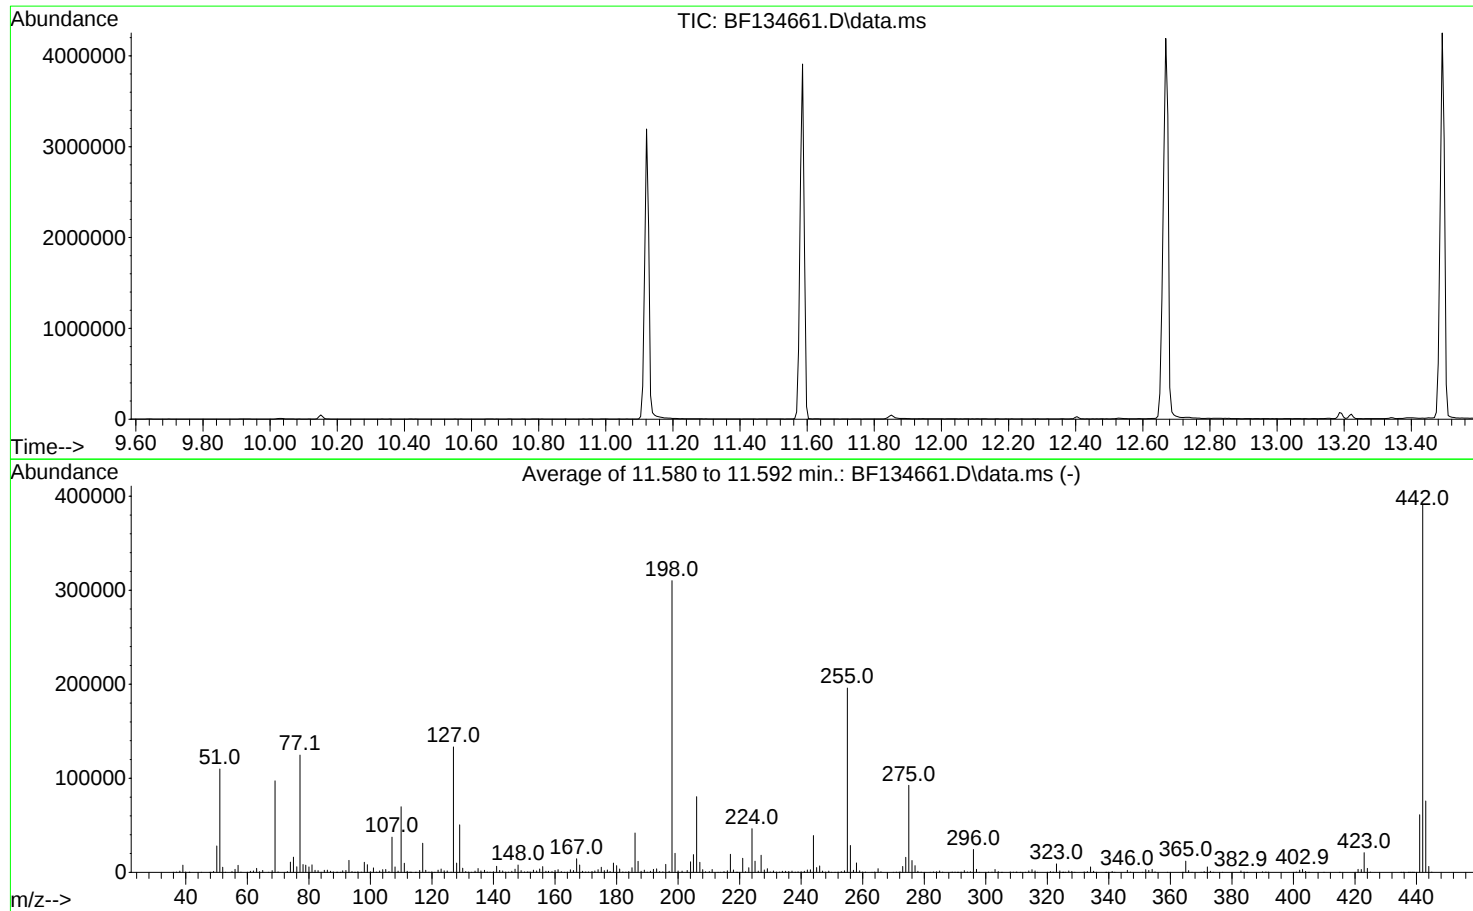




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	109936	PASS
68	69	0.00	2	2.0	1919	PASS
69	198	0.00	100	31.4	97376	PASS
70	69	0.00	2	0.5	534	PASS
127	198	10	80	43.0	133477	PASS
197	198	0.00	2	0.4	1237	PASS
198	198	100	100	100.0	310187	PASS
199	198	5	9	6.5	20217	PASS
275	198	10	60	29.8	92541	PASS
365	198	1	100	3.8	11893	PASS
441	198	0.01	100	19.8	61323	PASS
442	442	50	100	100.0	391147	PASS
443	442	15	24	19.4	75955	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080823\
Data File : BF134661.D
Acq On : 08 Aug 2023 08:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 08 08:33:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

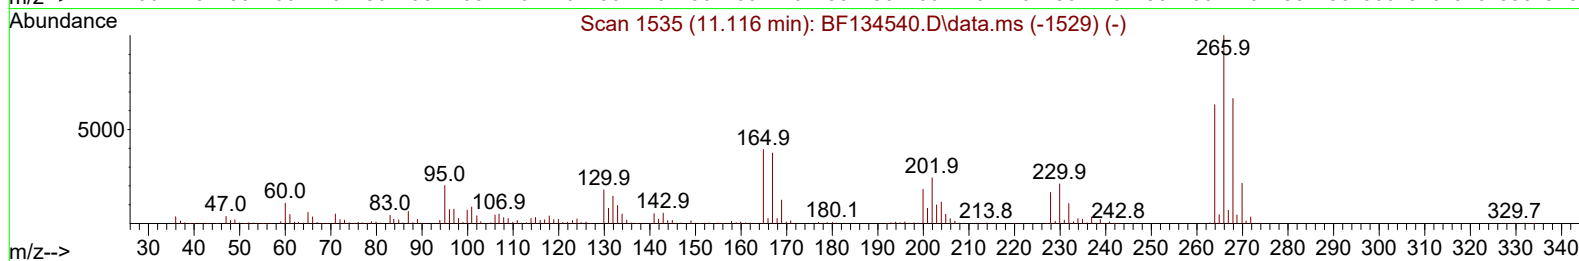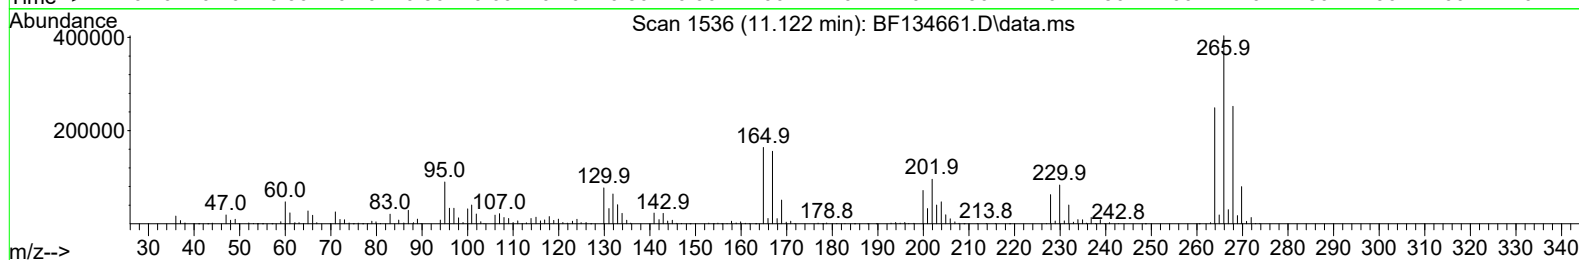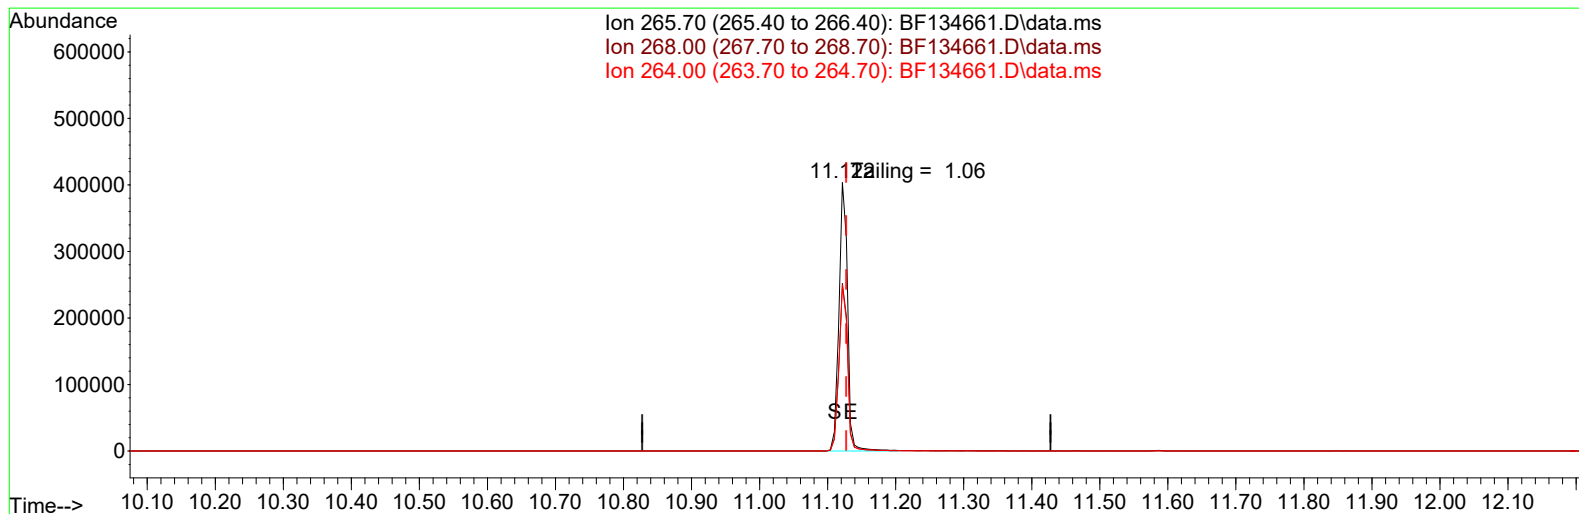

TIC: BF134661.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.006) 786971.86 ng




response 354856

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.45
264.00	59.70	61.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080823\
Data File : BF134661.D
Acq On : 08 Aug 2023 08:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 08 08:33:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

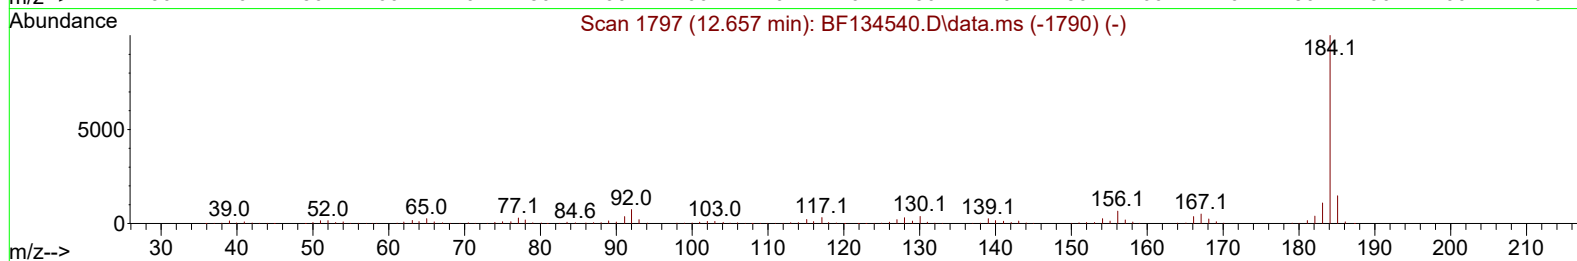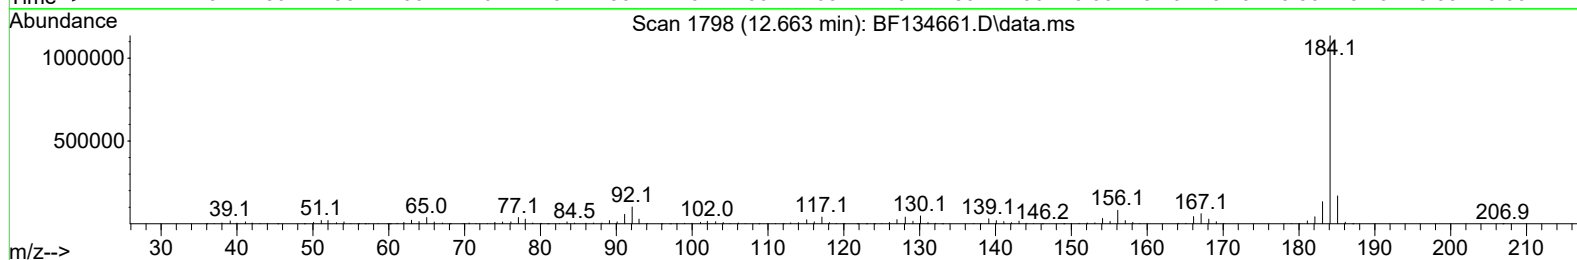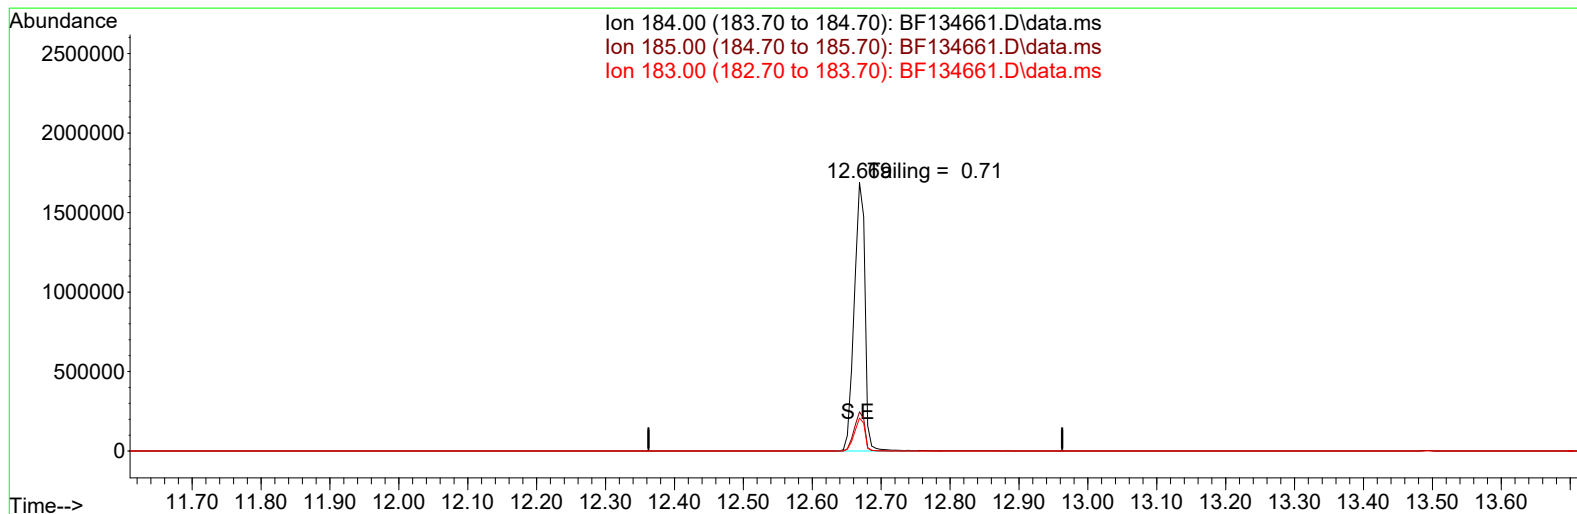

TIC: BF134661.D\data.ms

(77) Benzidine

12.663min (-12.663) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.00	0.00#
183.00	10.80	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/8/2023	BNA_F	<u>BF134661.D</u>
Compound Name	Response	Retention Time
DDT	767767	13.492
DDD	19126	13.192
DDE	448	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19574	787341	2.49

Instrument :
BNA_F
ClientSampleId :
DFTPP