


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080919\
 Data File : BF116116.D
 Acq On : 9 Aug 2019 17:01
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

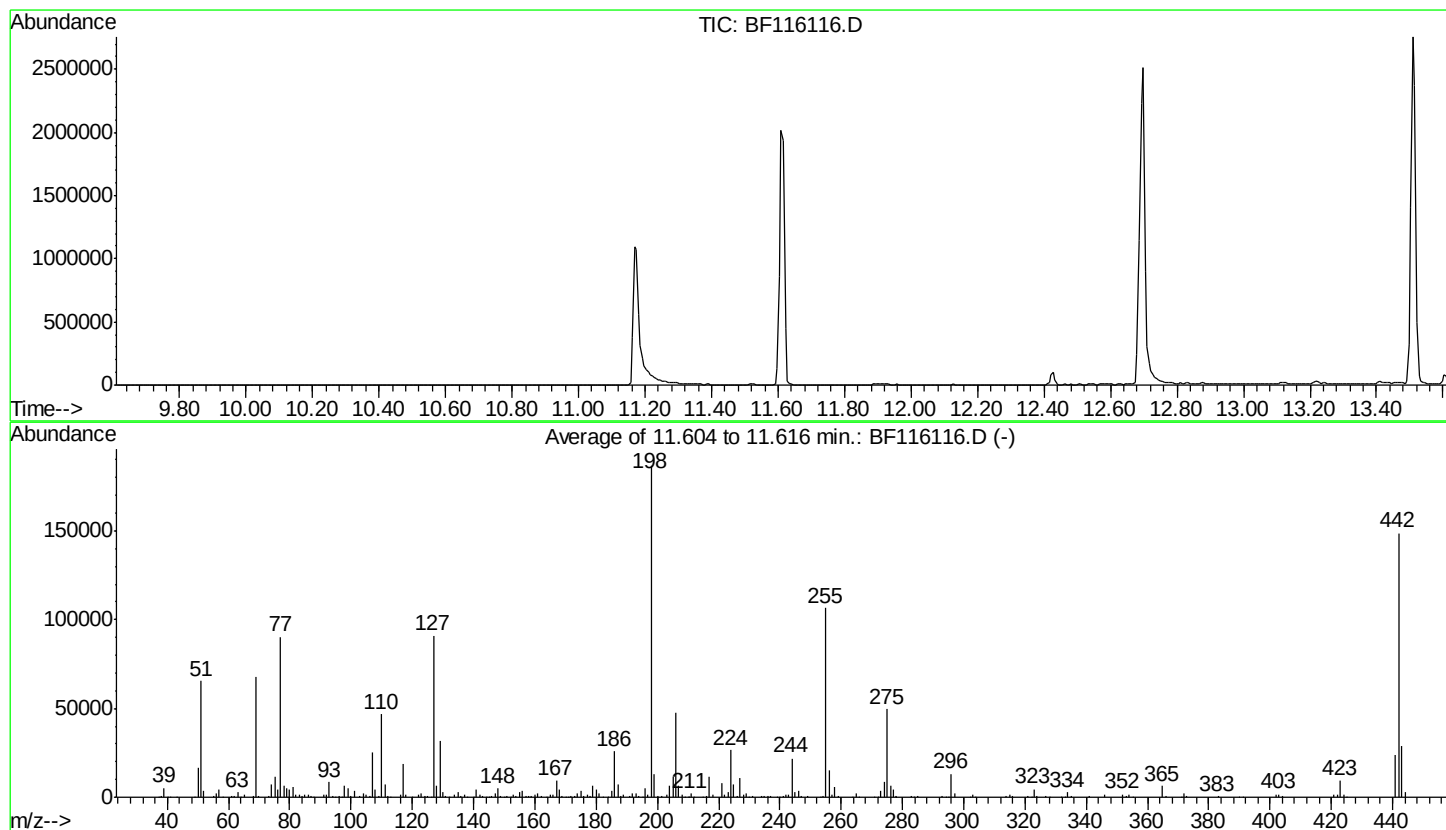

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	65440	PASS
68	69	0.00	2	1.6	1098	PASS
69	198	0.00	100	36.3	67696	PASS
70	69	0.00	2	0.6	385	PASS
127	198	10	80	48.7	90997	PASS
197	198	0.00	2	0.6	1131	PASS
198	198	100	100	100.0	186674	PASS
199	198	5	9	6.9	12848	PASS
275	198	10	60	26.5	49504	PASS
365	198	1	100	3.3	6180	PASS
441	198	0.01	100	12.7	23797	PASS
442	198	50	100	79.6	148597	PASS
443	442	15	24	19.4	28843	PASS