
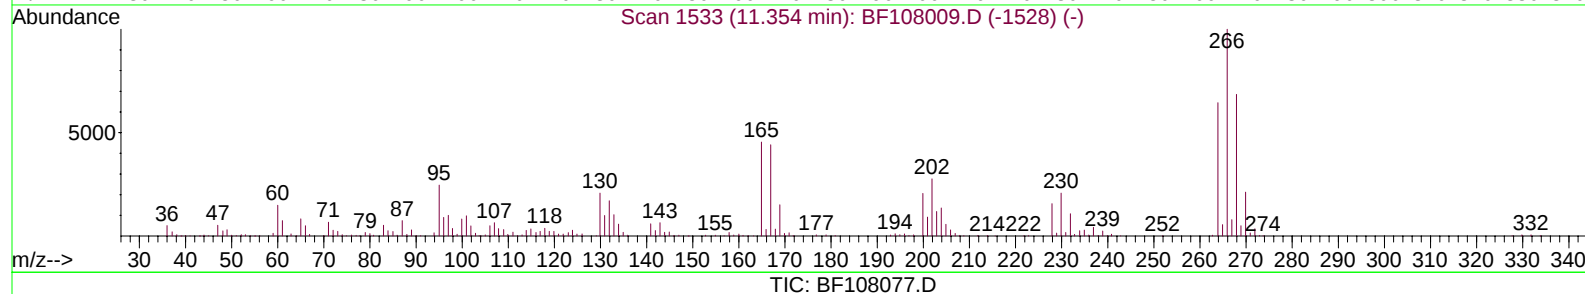
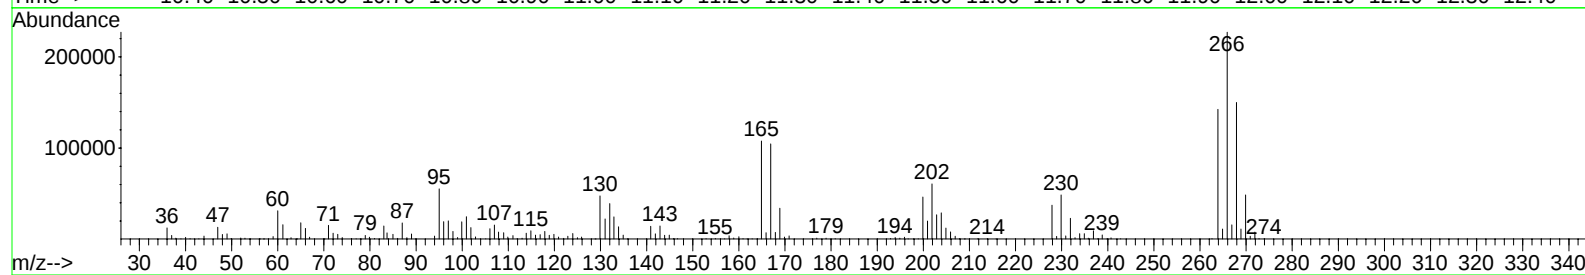


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081018\
Data File : BF108077.D
Acq On : 10 Aug 2018 12:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 19:11:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

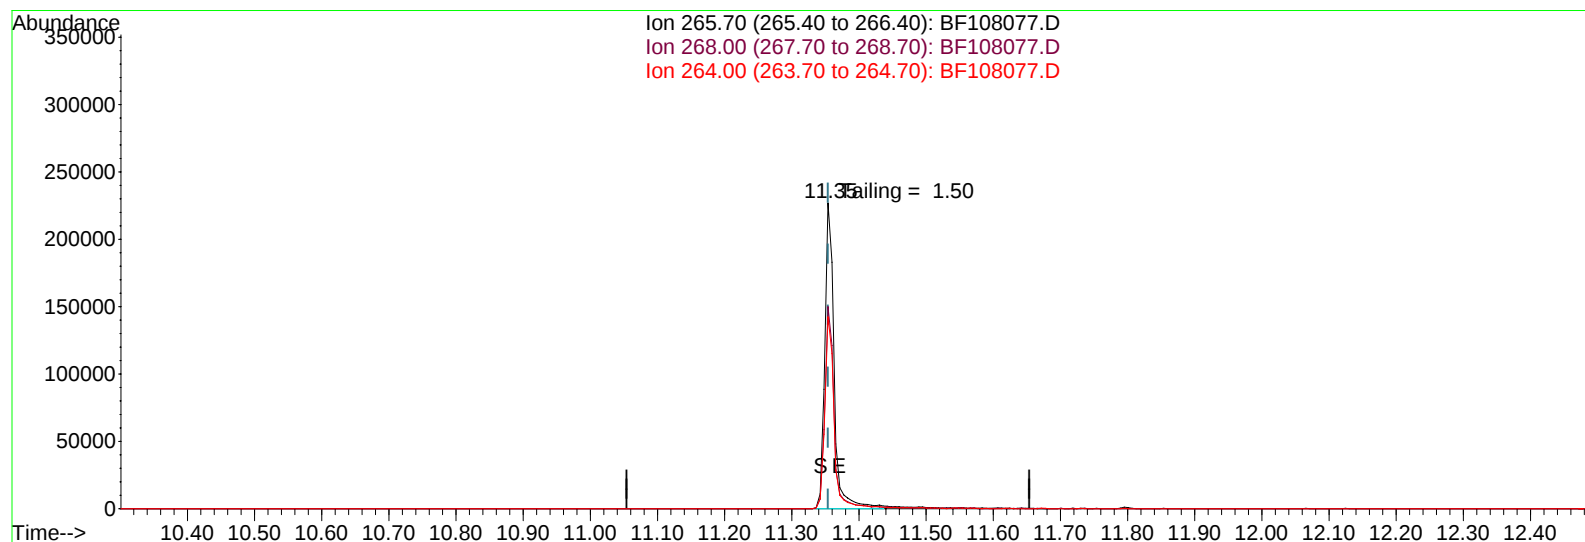

(69) Pentachlorophenol (C)




11.354min (+0.000) 72894.28ng

response 223806

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.10
264.00	61.90	62.77
0.00	0.00	0.00

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081018\  
Data File   : BF108077.D  
Acq On      : 10 Aug 2018   12:09  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Aug 10 19:11:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

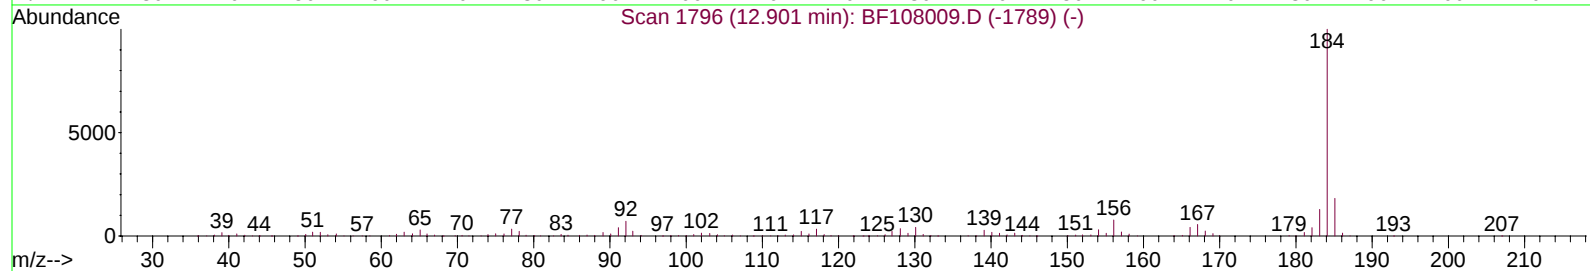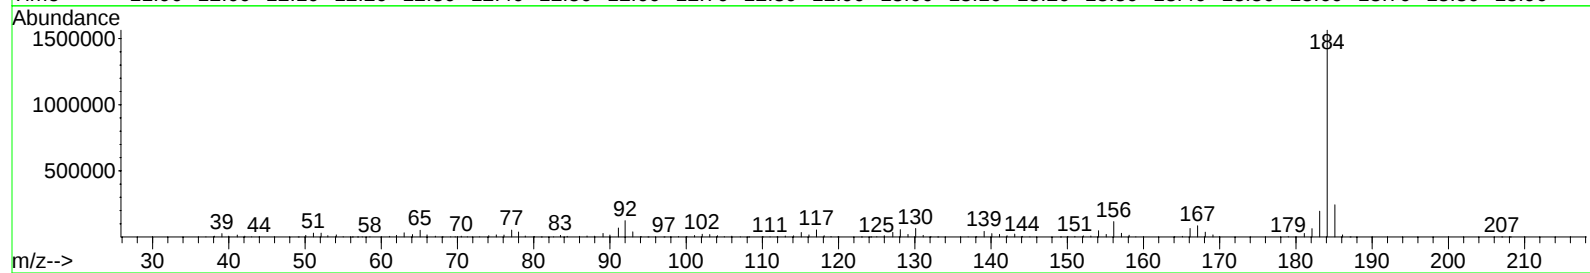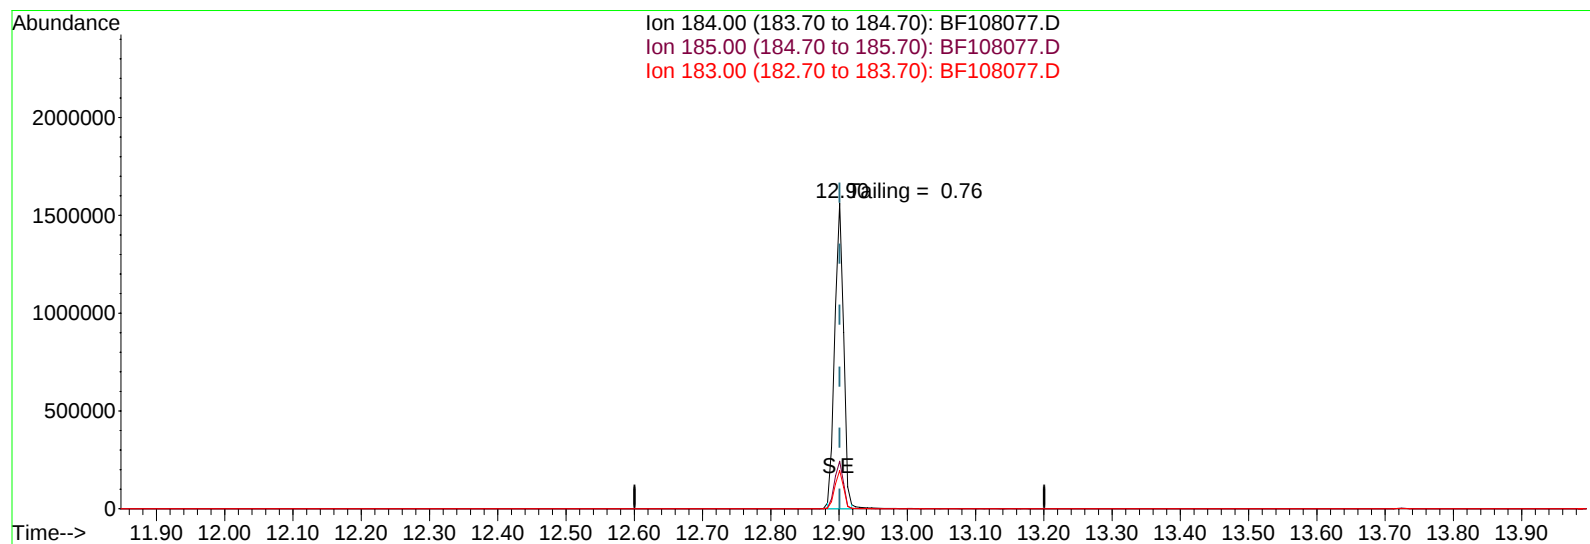

TIC: BF108077.D

(76) Benzidine

12.901min (+0.000) 57104.66ng

```
response 1418824
```

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.55
183.00	11.60	12.49
0.00	0.00	0.00