


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081018\
 Data File : BF108077.D
 Acq On : 10 Aug 2018 12:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 12:24:24 2018

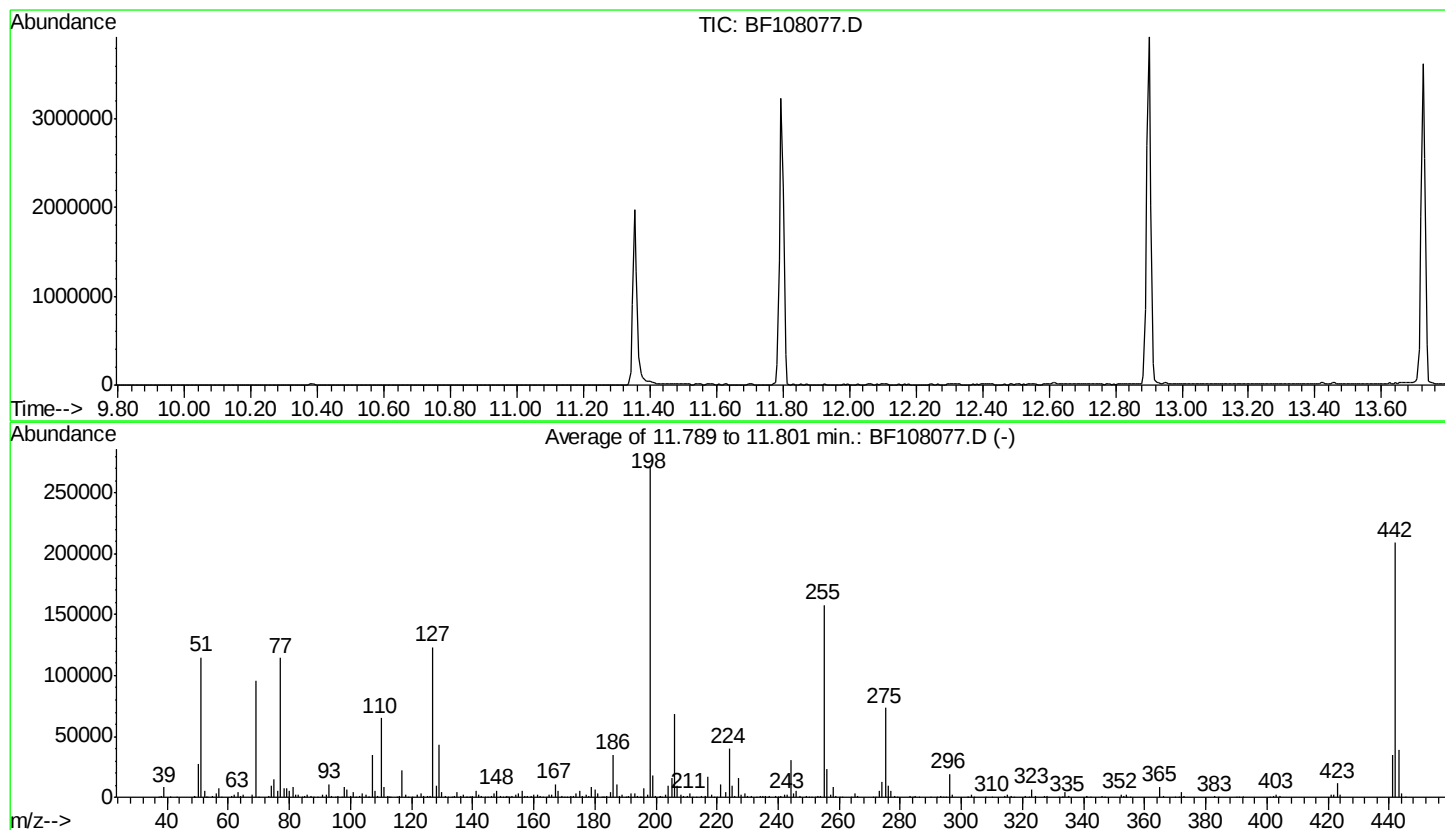

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	114850	PASS
68	69	0.00	2	1.8	1695	PASS
69	198	0.00	100	35.1	95762	PASS
70	69	0.00	2	0.5	449	PASS
127	198	10	80	45.2	123272	PASS
197	198	0.00	2	0.6	1676	PASS
198	198	100	100	100.0	272576	PASS
199	198	5	9	6.7	18378	PASS
275	198	10	60	26.9	73285	PASS
365	198	1	100	3.2	8617	PASS
441	198	0.01	100	12.8	34990	PASS
442	198	50	100	76.8	209330	PASS
443	442	15	24	18.6	39002	PASS