


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081018\
Data File : BF108104.D
Acq On : 11 Aug 2018 00:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 08 12:24:24 2018

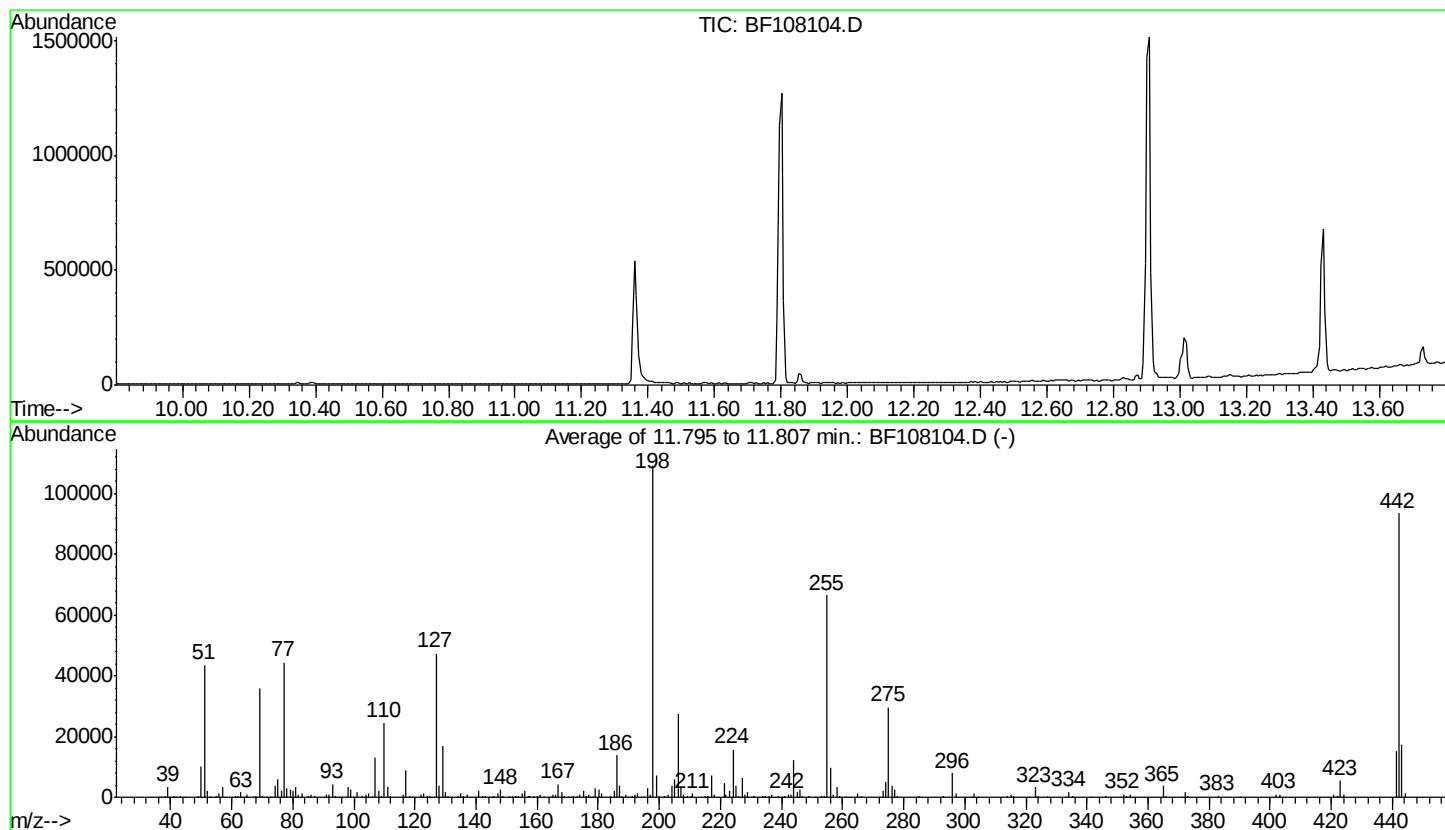

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	43558	PASS
68	69	0.00	2	1.8	642	PASS
69	198	0.00	100	32.7	35696	PASS
70	69	0.00	2	0.8	288	PASS
127	198	10	80	43.3	47332	PASS
197	198	0.00	2	0.7	735	PASS
198	198	100	100	100.0	109194	PASS
199	198	5	9	6.5	7096	PASS
275	198	10	60	27.2	29650	PASS
365	198	1	100	3.3	3654	PASS
441	198	0.01	100	13.9	15146	PASS
442	198	50	100	85.6	93445	PASS
443	442	15	24	18.5	17302	PASS