


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081019\
 Data File : BF116140.D
 Acq On : 10 Aug 2019 10:00
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

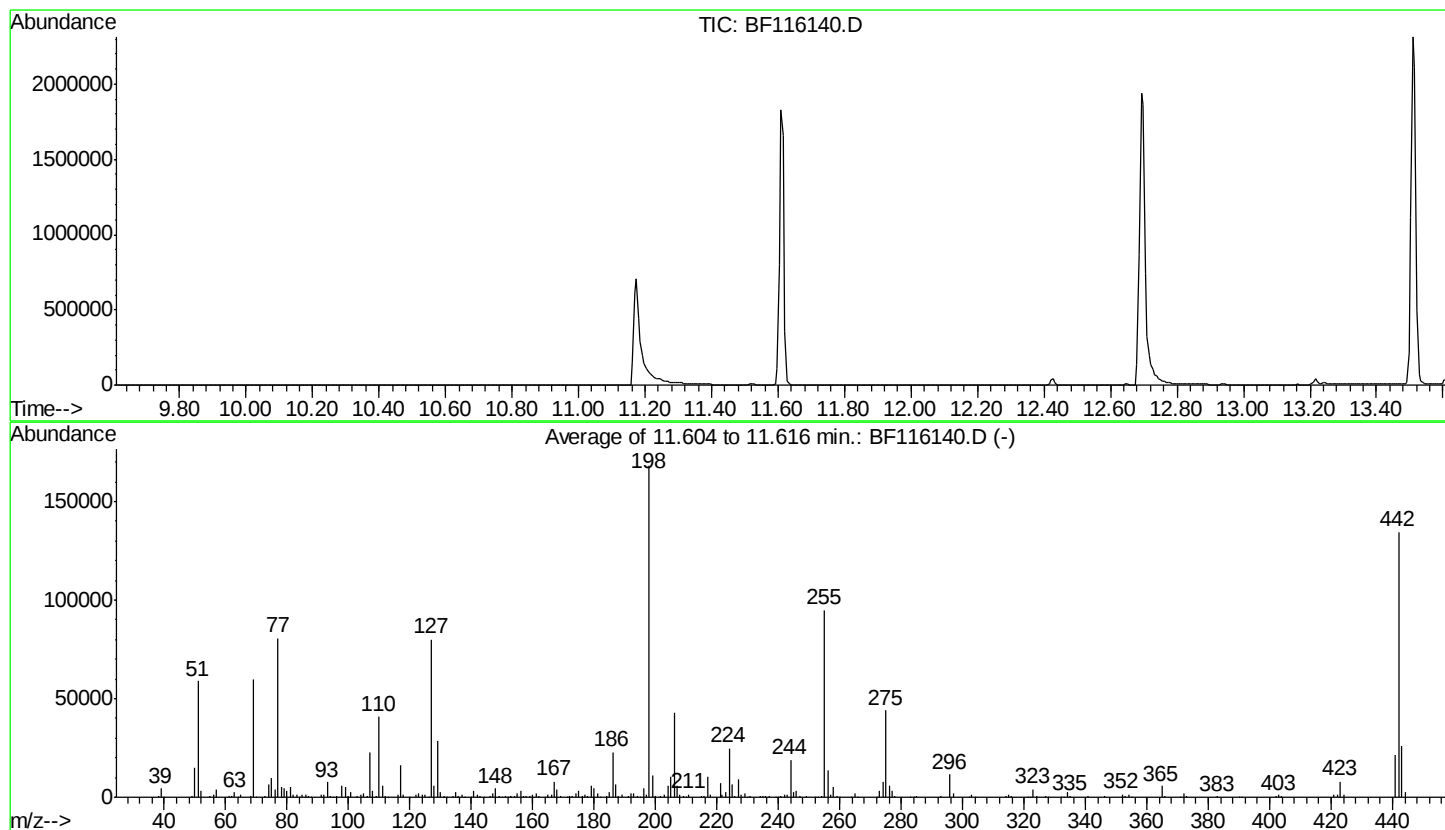

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	58904	PASS
68	69	0.00	2	1.6	935	PASS
69	198	0.00	100	35.6	59962	PASS
70	69	0.00	2	0.5	289	PASS
127	198	10	80	47.6	80117	PASS
197	198	0.00	2	0.6	1065	PASS
198	198	100	100	100.0	168240	PASS
199	198	5	9	6.7	11234	PASS
275	198	10	60	26.2	44101	PASS
365	198	1	100	3.3	5572	PASS
441	198	0.01	100	12.8	21520	PASS
442	198	50	100	80.1	134730	PASS
443	442	15	24	19.4	26096	PASS