
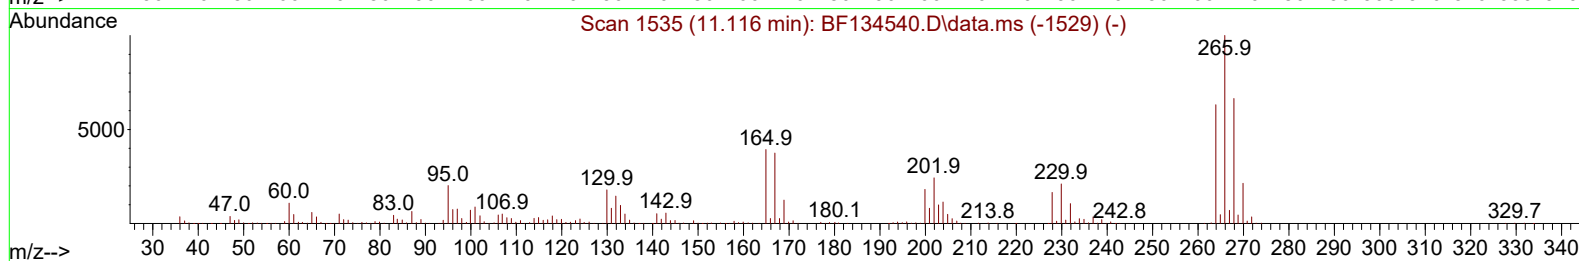
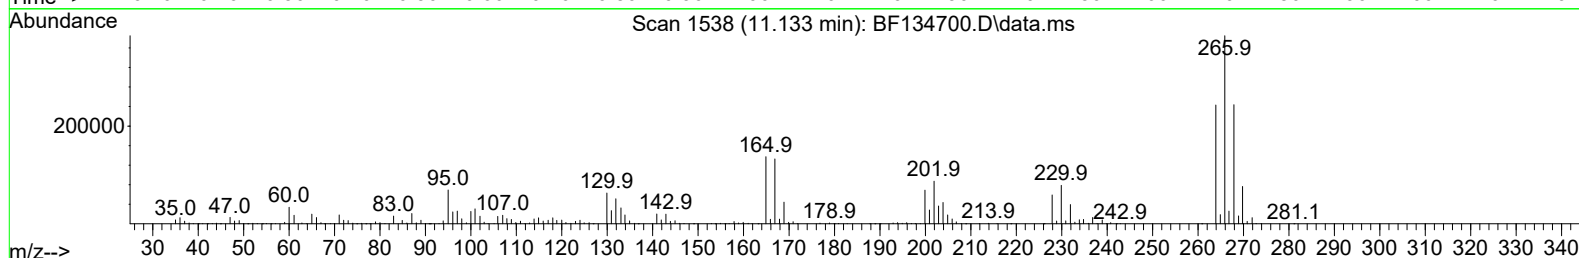


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081023\
Data File : BF134700.D
Acq On : 10 Aug 2023 09:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 05:07:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

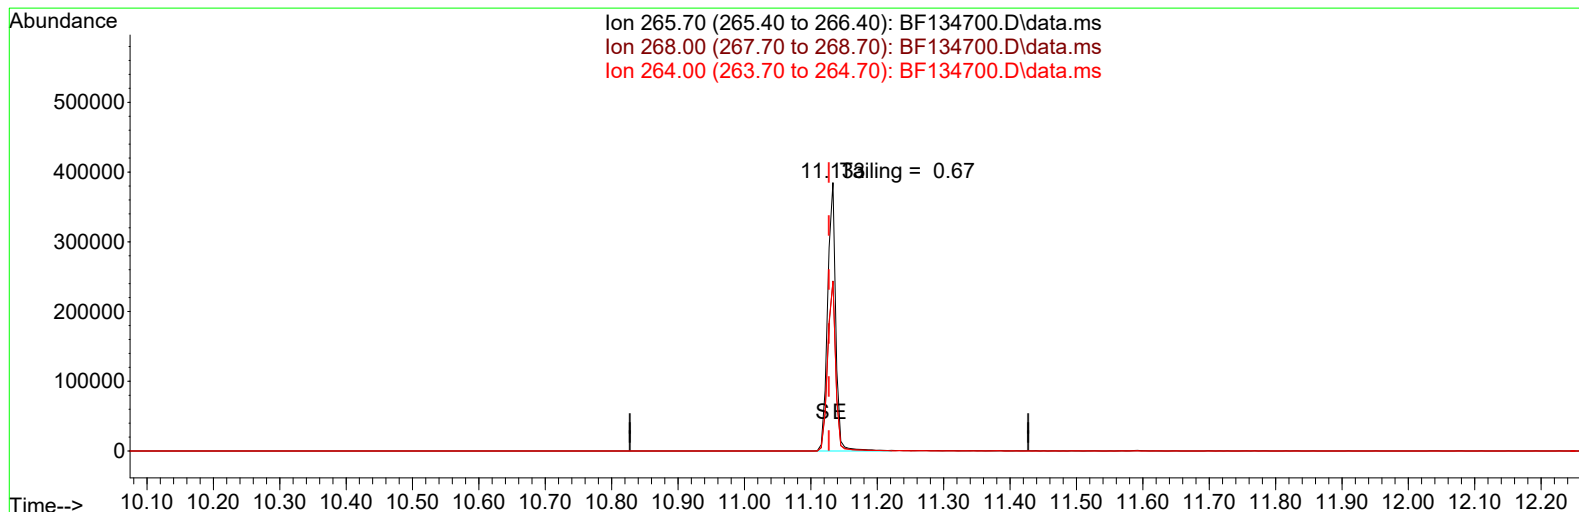

TIC: BF134700.D\data.ms

(70) Pentachlorophenol (C)




11.133min (+ 0.006) 615220.05 ng

response 330251

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.35
264.00	59.70	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081023\
Data File : BF134700.D
Acq On : 10 Aug 2023 09:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 05:07:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

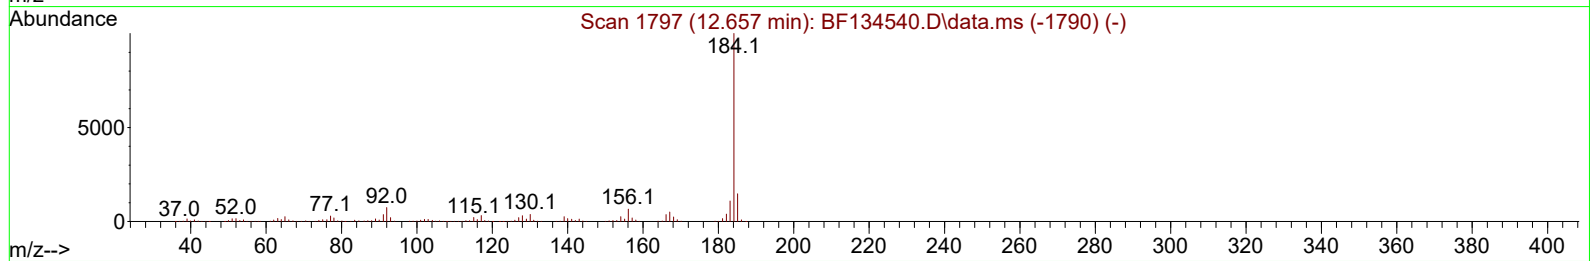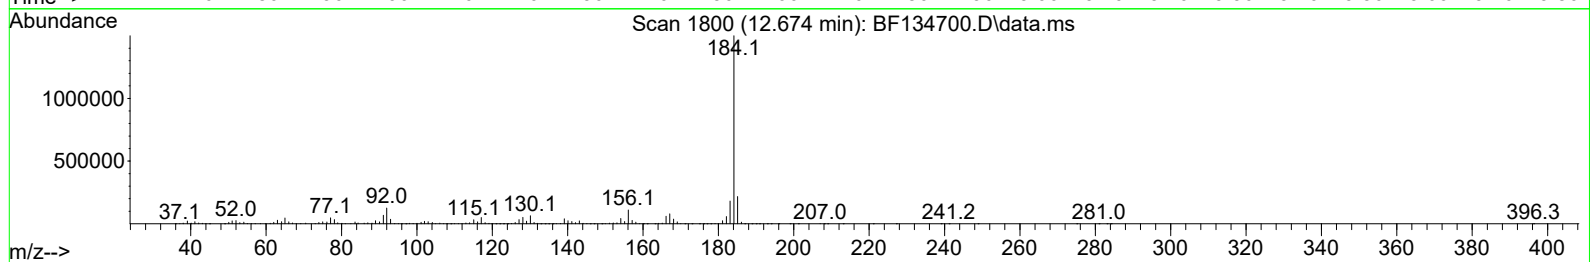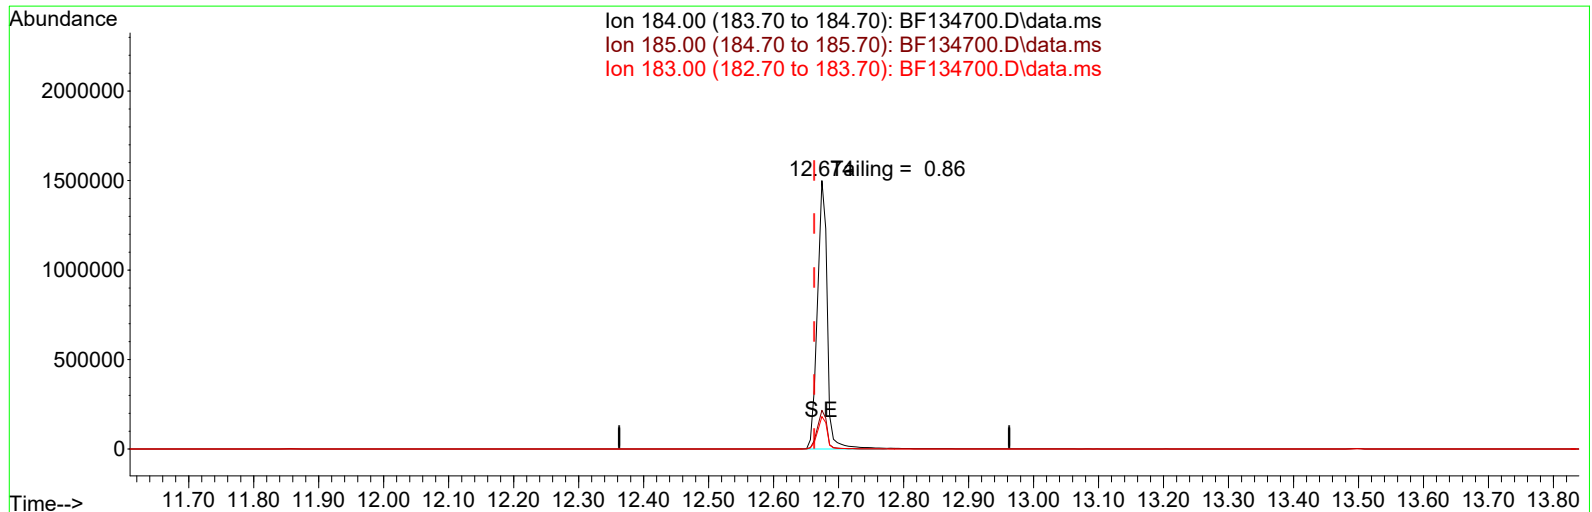

TIC: BF134700.D\data.ms

(77) Benzidine**12.674min (+ 0.012) 107038.46 ng****response 1575386**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.44
183.00	10.80	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/10/2023	BNA_F	<u>BF134700.D</u>
Compound Name	Response	Retention Time
DDT	740911	13.498
DDD	23164	13.198
DDE	1254	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24418	765329	3.19