
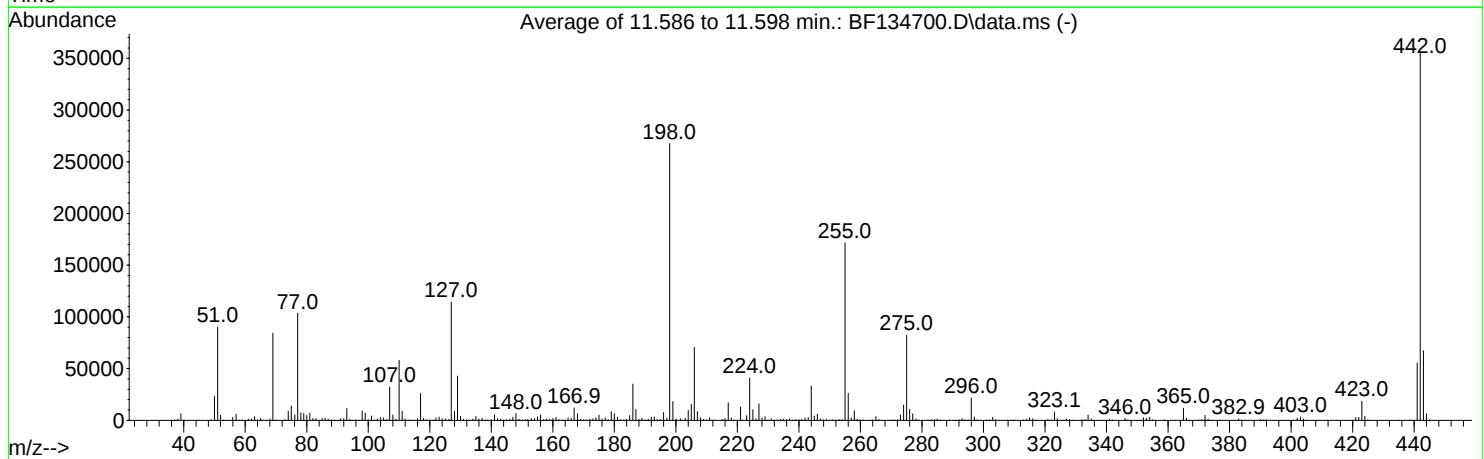


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081023\
Data File : BF134700.D
Acq On : 10 Aug 2023 09:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 04 09:29:15 2023

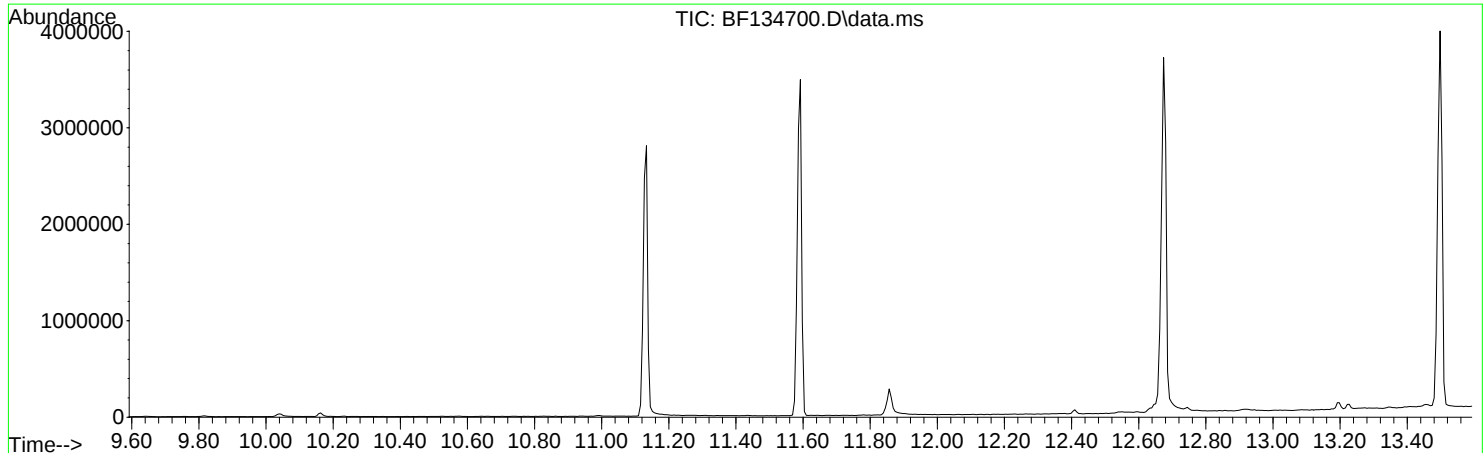




AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	90187	PASS
68	69	0.00	2	1.7	1402	PASS
69	198	0.00	100	31.5	84302	PASS
70	69	0.00	2	0.4	354	PASS
127	198	10	80	42.8	114456	PASS
197	198	0.00	2	0.8	2154	PASS
198	198	100	100	100.0	267549	PASS
199	198	5	9	6.8	18179	PASS
275	198	10	60	30.8	82304	PASS
365	198	1	100	4.3	11624	PASS
441	198	0.01	100	20.7	55448	PASS
442	442	50	100	100.0	355712	PASS
443	442	15	24	18.9	67240	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081023\
Data File : BF134700.D
Acq On : 10 Aug 2023 09:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 11 05:07:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

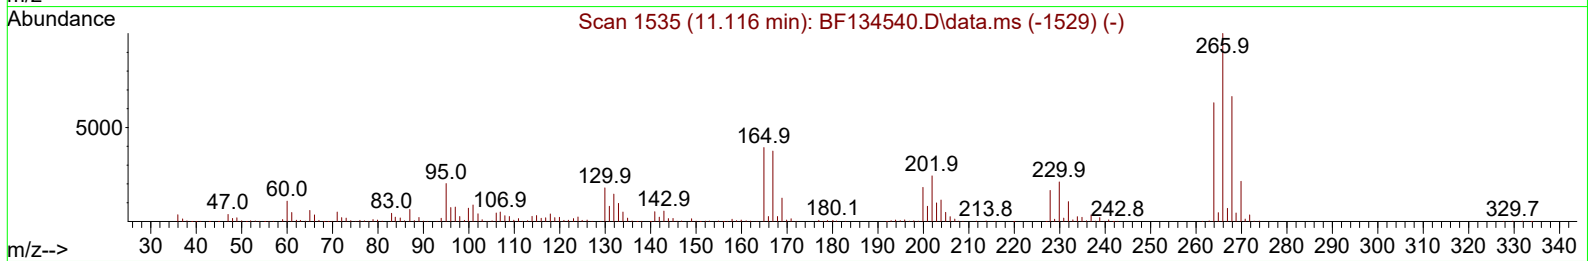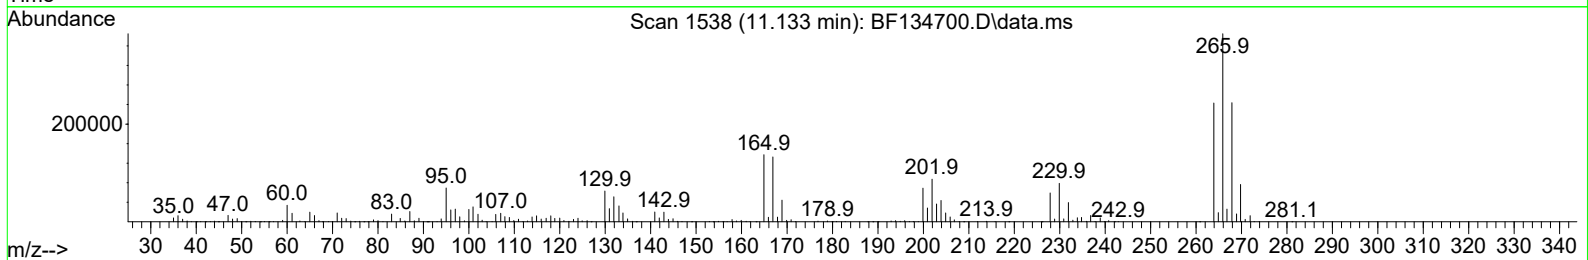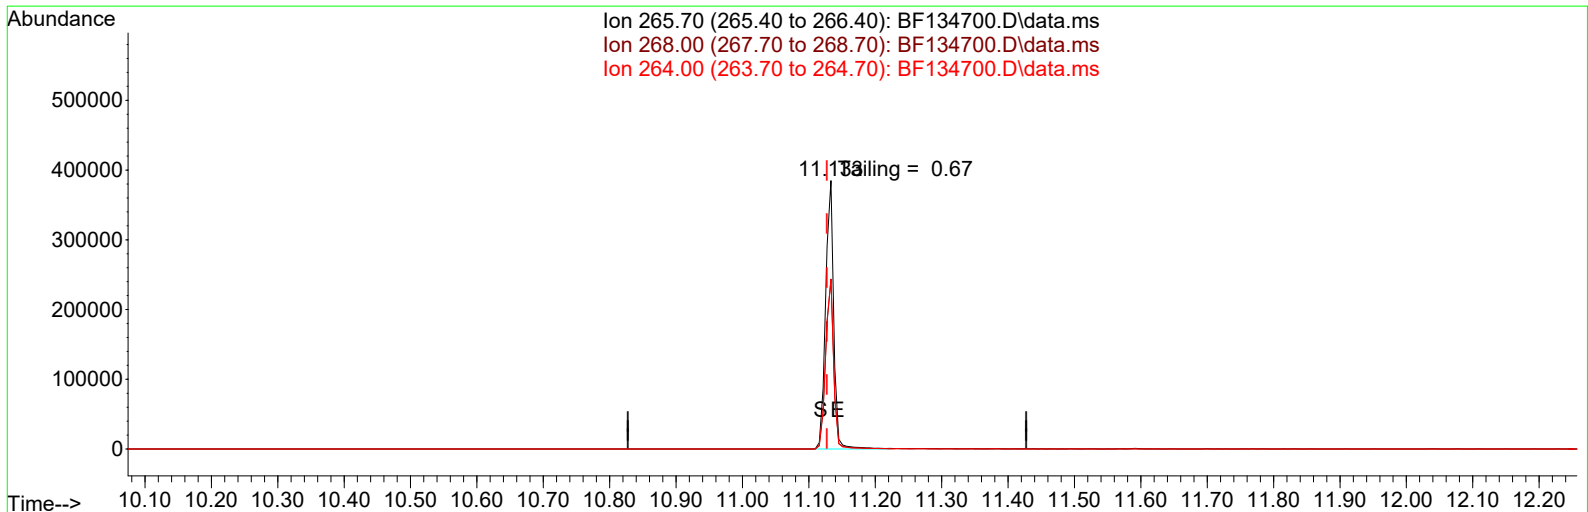

TIC: BF134700.D\data.ms

(70) Pentachlorophenol (C)

11.133min (+ 0.006) 615220.05 ng




response 330251

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.35
264.00	59.70	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081023\
Data File : BF134700.D
Acq On : 10 Aug 2023 09:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 11 05:07:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

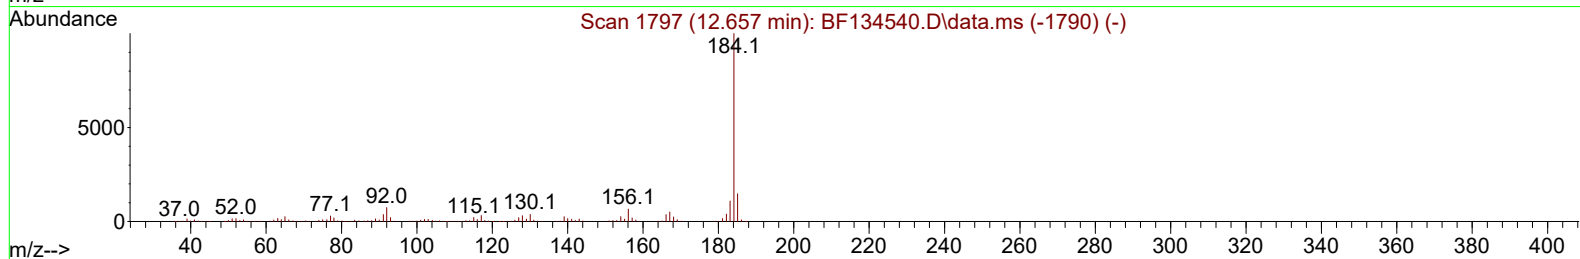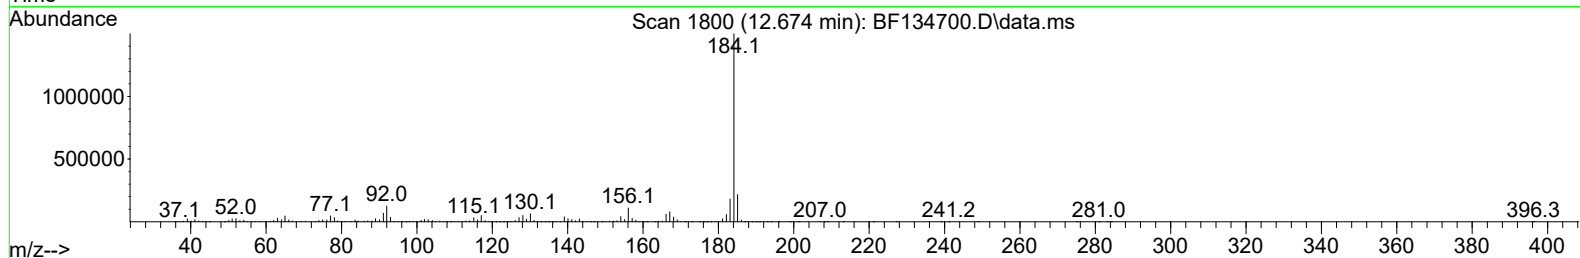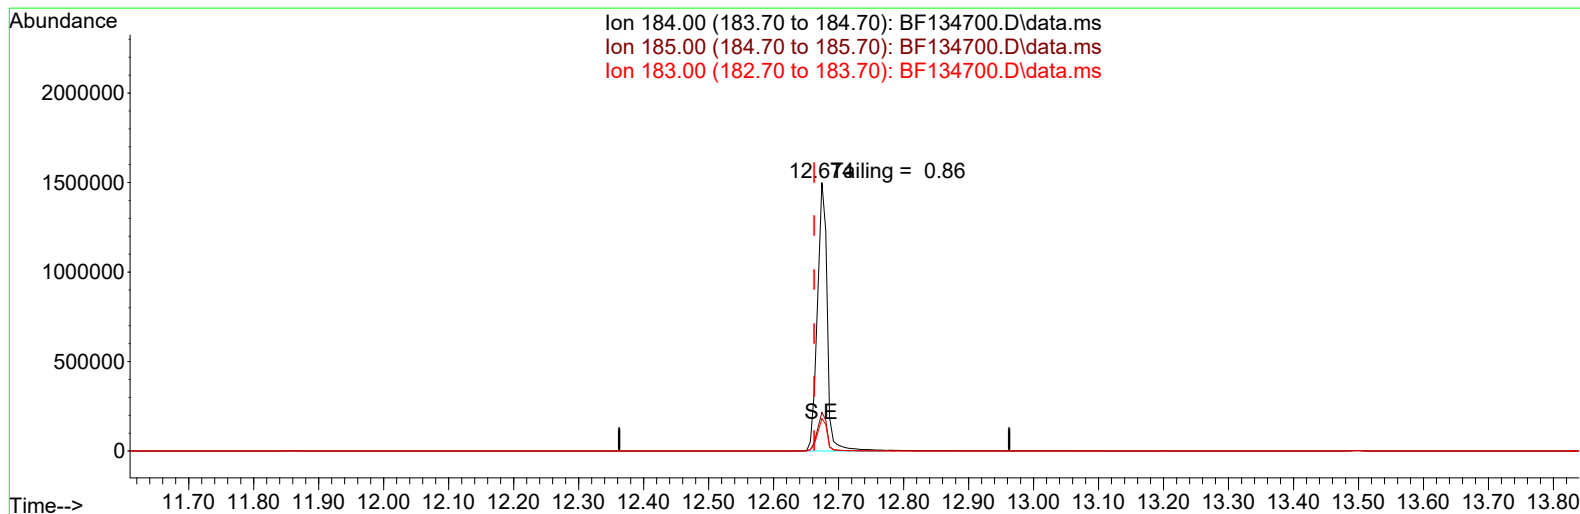

TIC: BF134700.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 107038.46 ng

response 1575386

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.44
183.00	10.80	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/10/2023	BNA_F	<u>BF134700.D</u>
Compound Name	Response	Retention Time
DDT	740911	13.498
DDD	23164	13.198
DDE	1254	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24418	765329	3.19

Instrument :
BNA_F
ClientSampleId :
DFTPP