
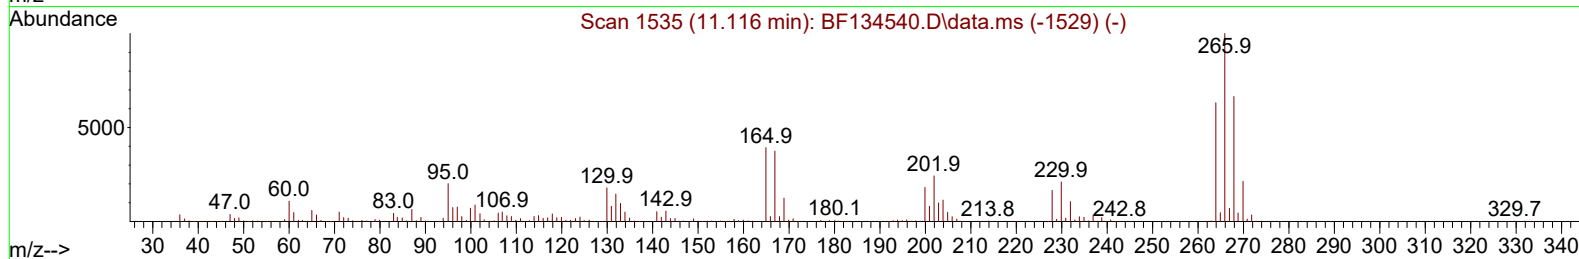
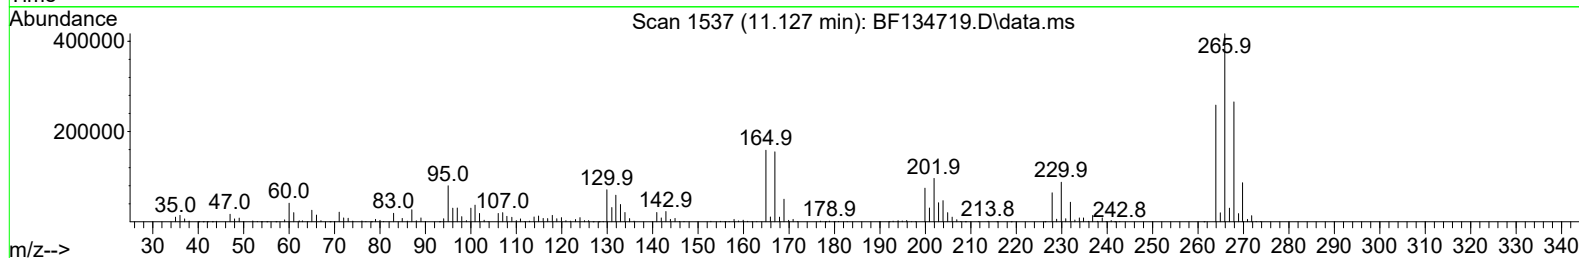


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081123\
Data File : BF134719.D
Acq On : 11 Aug 2023 07:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 00:46:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

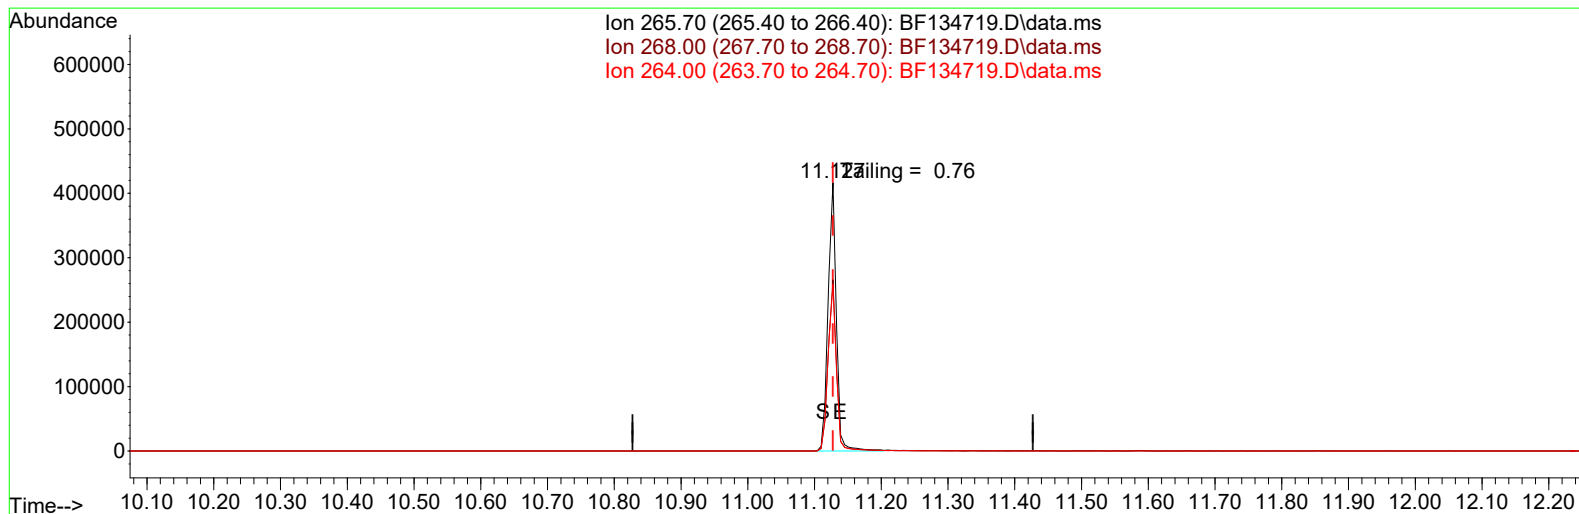

TIC: BF134719.D\data.ms

(70) Pentachlorophenol (C)




11.127min (+ 0.000) 528589.61 ng

response 363197

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.80
264.00	59.70	62.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081123\
Data File : BF134719.D
Acq On : 11 Aug 2023 07:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 00:46:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

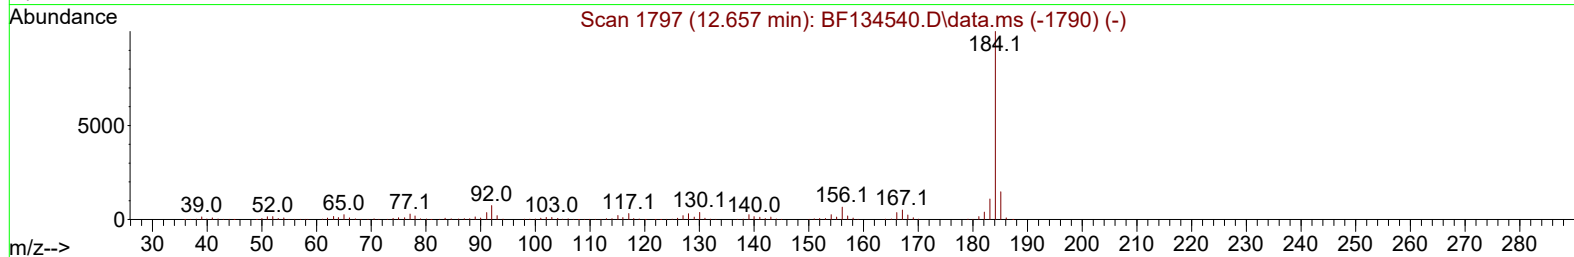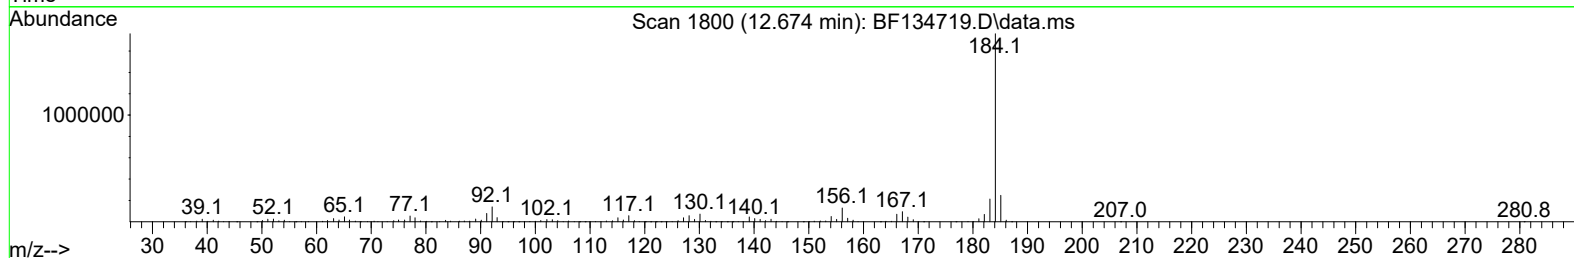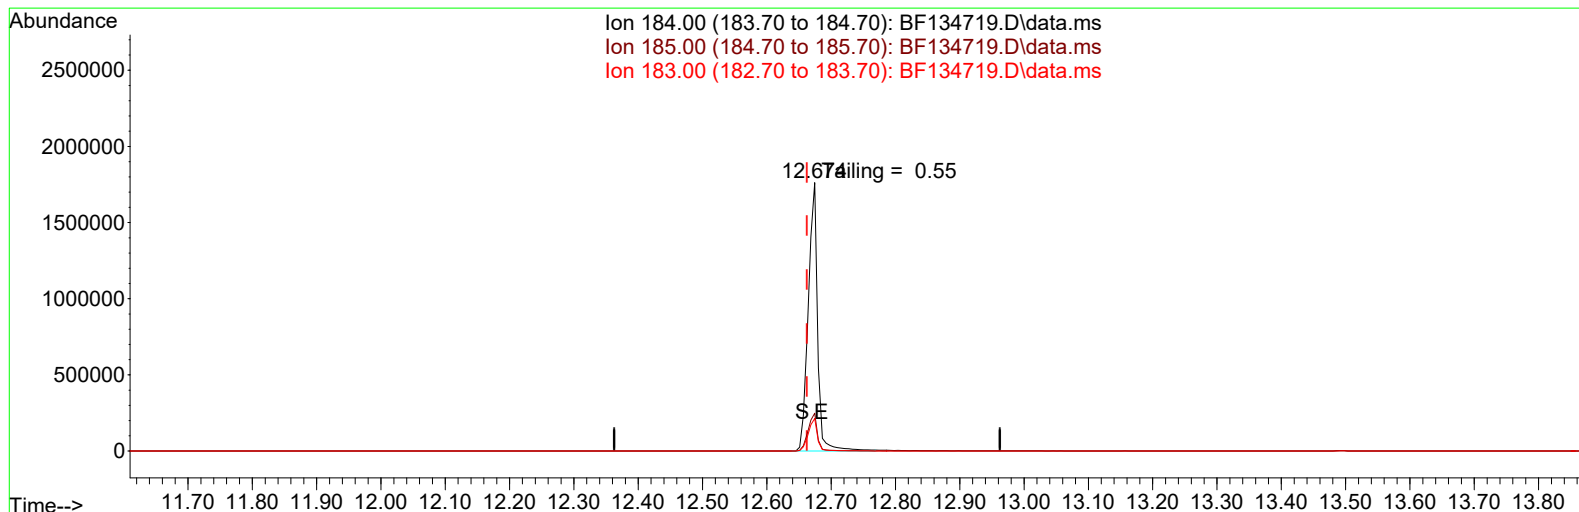

TIC: BF134719.D\data.ms

(77) Benzidine**12.674min (+ 0.012) 194871.19 ng****response 1810543**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.09
183.00	10.80	12.12
0.00	0.00	0.00