
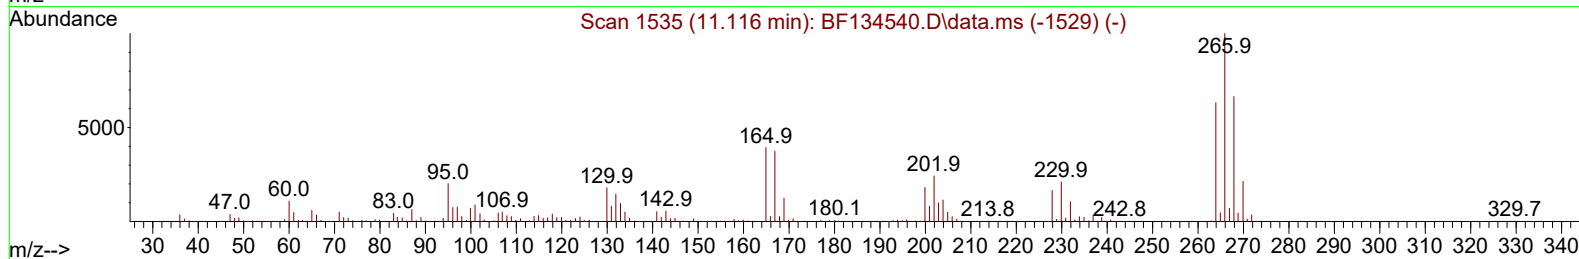
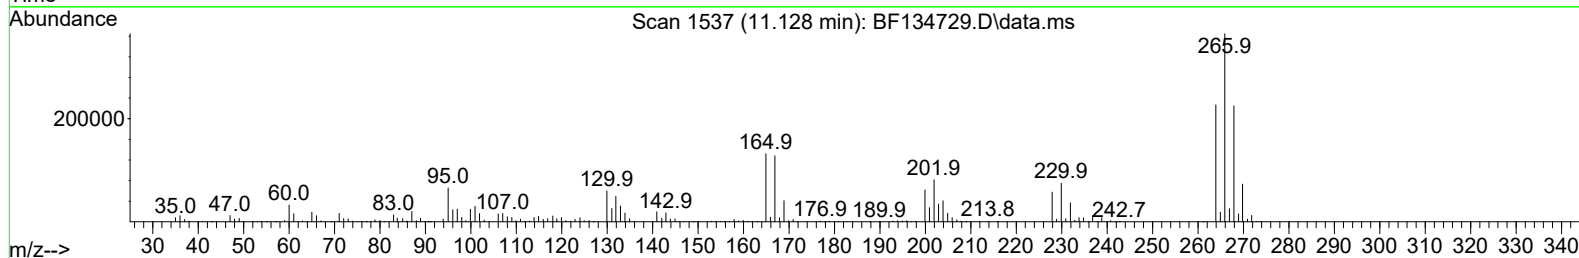


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081123\
Data File : BF134729.D
Acq On : 11 Aug 2023 13:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 00:47:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

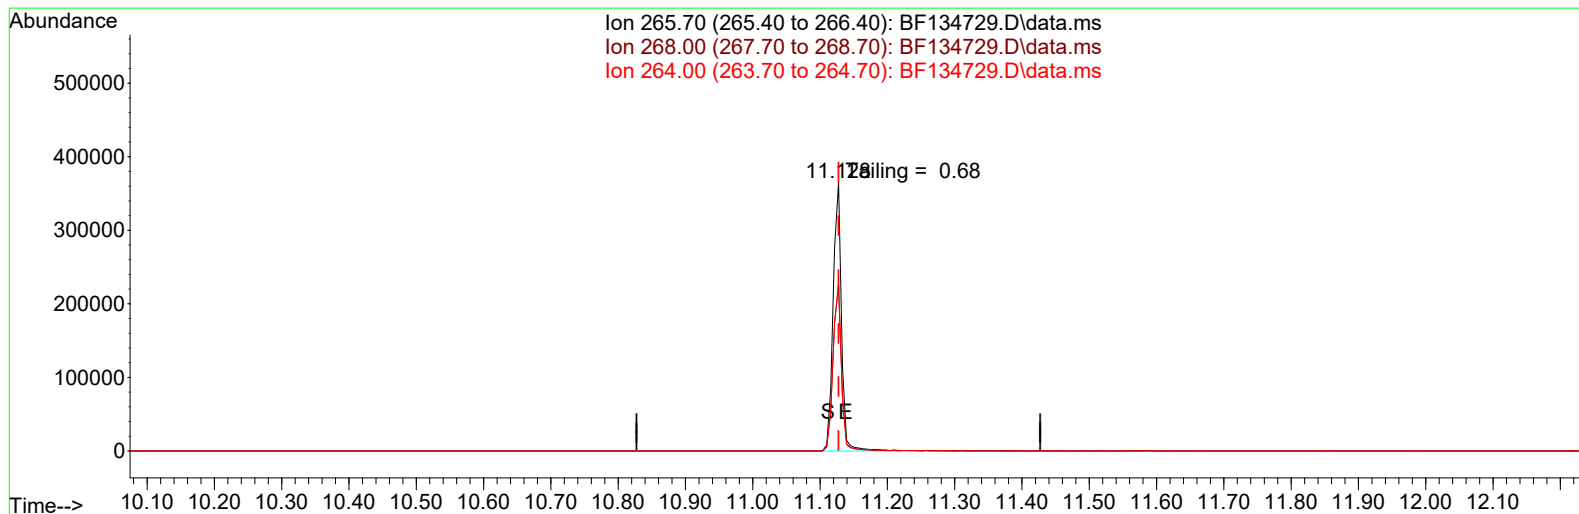

TIC: BF134729.D\data.ms

(70) Pentachlorophenol (C)




11.128min (+ 0.000) 275954.00 ng

response 316016

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	61.71
264.00	59.70	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081123\
Data File : BF134729.D
Acq On : 11 Aug 2023 13:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 00:47:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

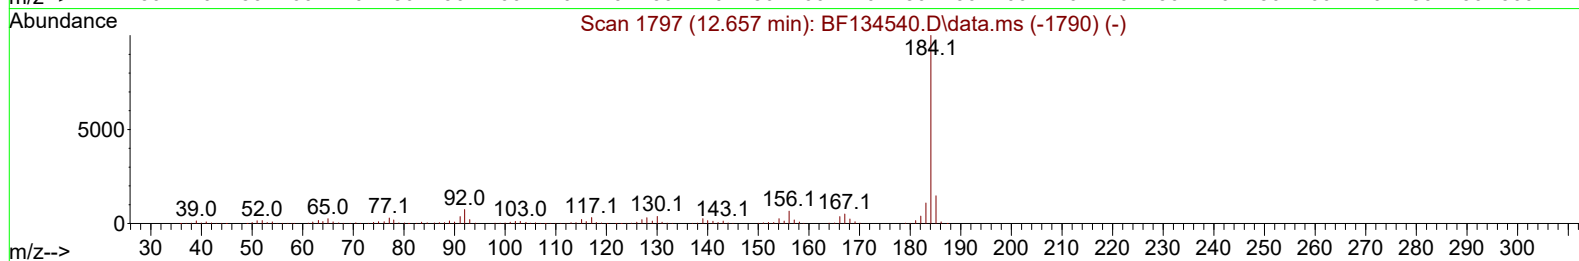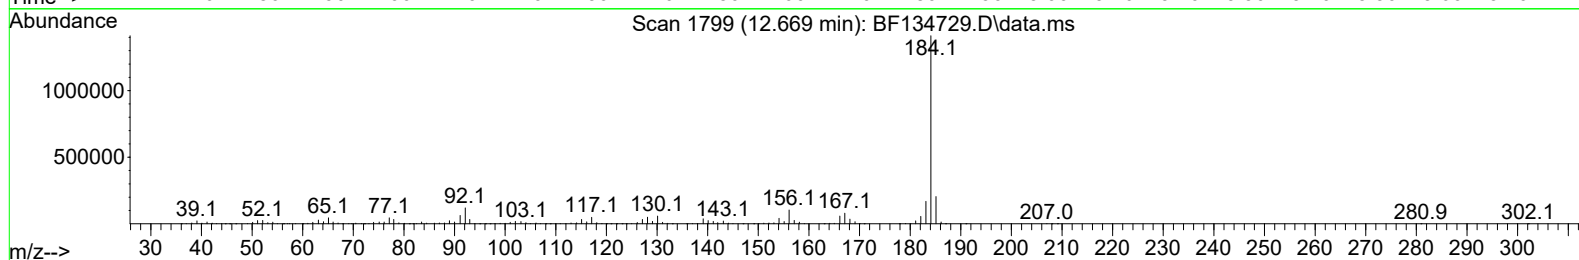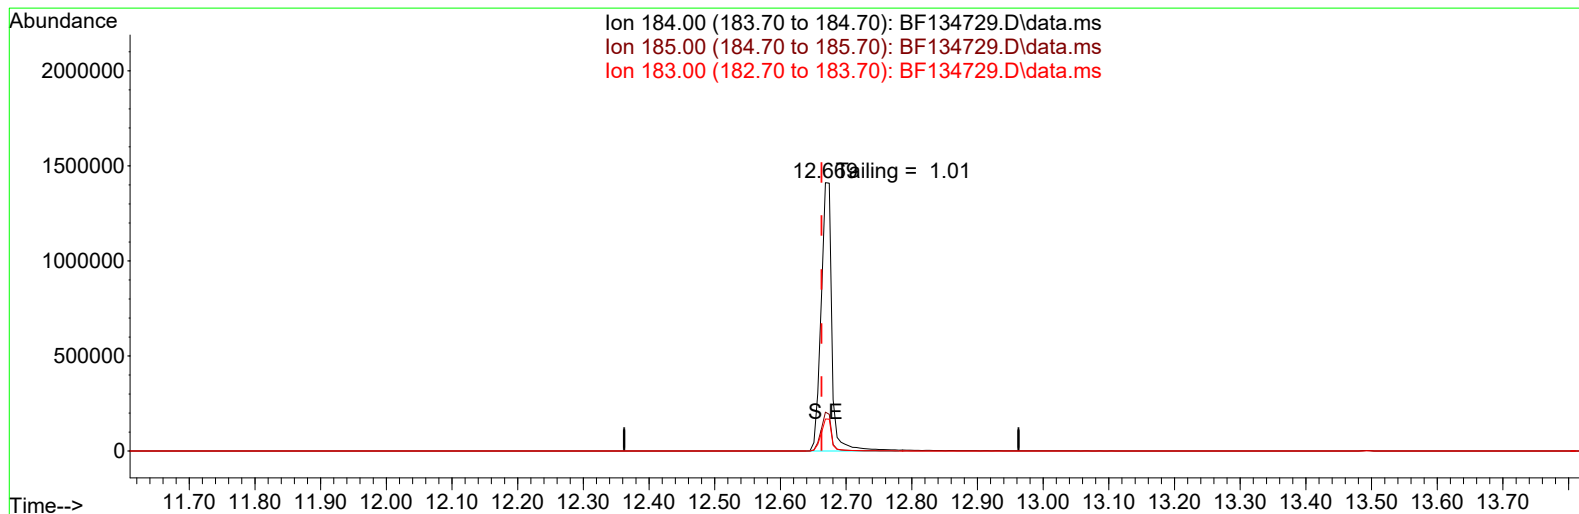

TIC: BF134729.D\data.ms

(77) Benzidine**12.669min (+ 0.006) 681340.74 ng****response 1626951**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.48
183.00	10.80	11.93
0.00	0.00	0.00