
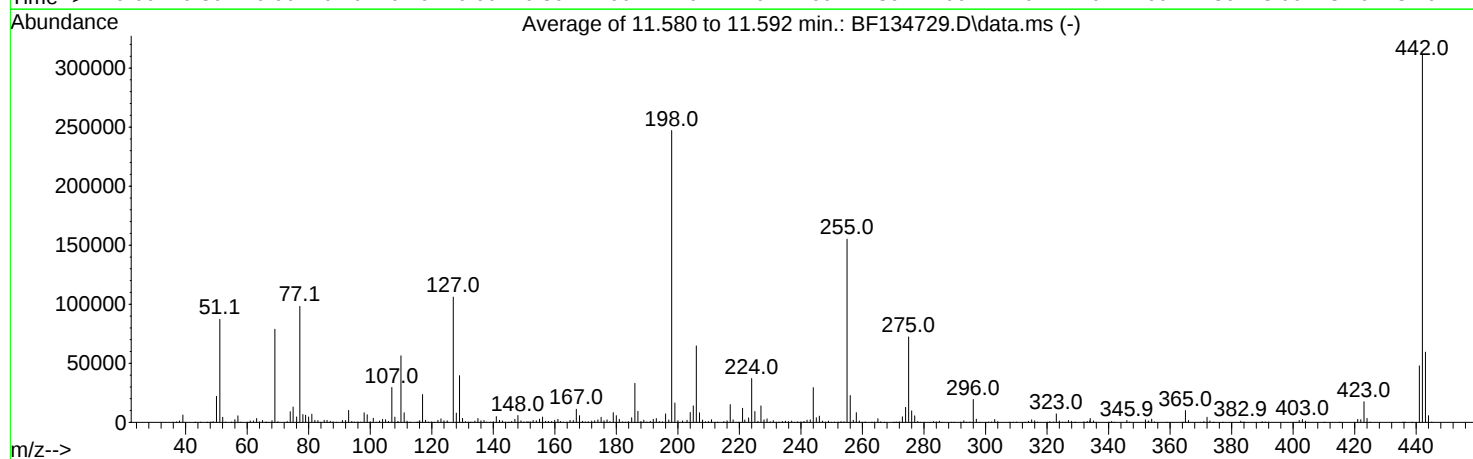


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081123\
 Data File : BF134729.D
 Acq On : 11 Aug 2023 13:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 04 09:29:15 2023



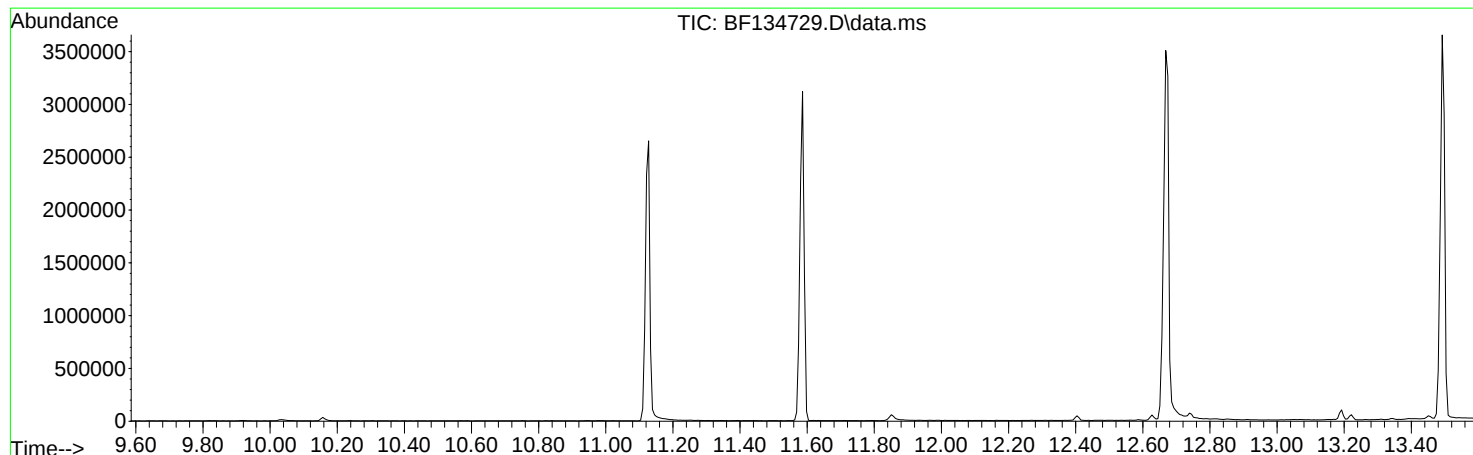


AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	87275	PASS
68	69	0.00	2	1.9	1491	PASS
69	198	0.00	100	31.9	78884	PASS
70	69	0.00	2	0.7	513	PASS
127	198	10	80	42.9	106123	PASS
197	198	0.00	2	0.8	2097	PASS
198	198	100	100	100.0	247125	PASS
199	198	5	9	6.7	16473	PASS
275	198	10	60	29.3	72325	PASS
365	198	1	100	4.1	10082	PASS
441	198	0.01	100	19.3	47776	PASS
442	442	50	100	100.0	311467	PASS
443	442	15	24	19.1	59432	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 12 00:47:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

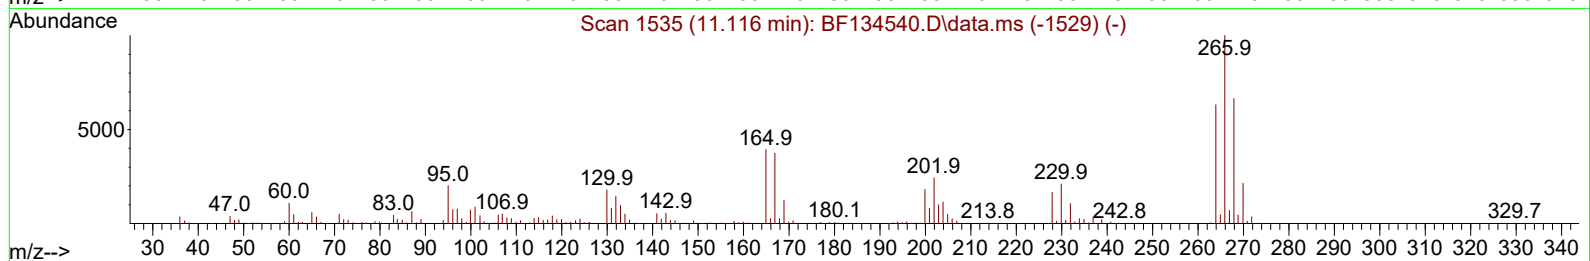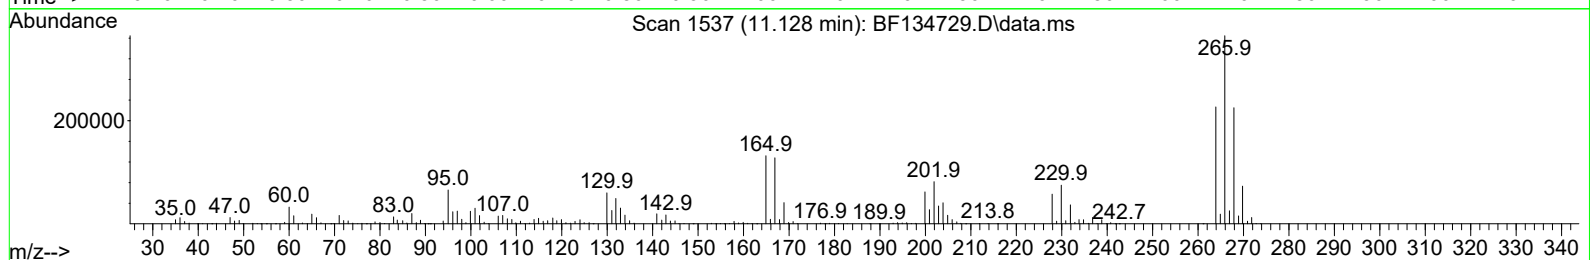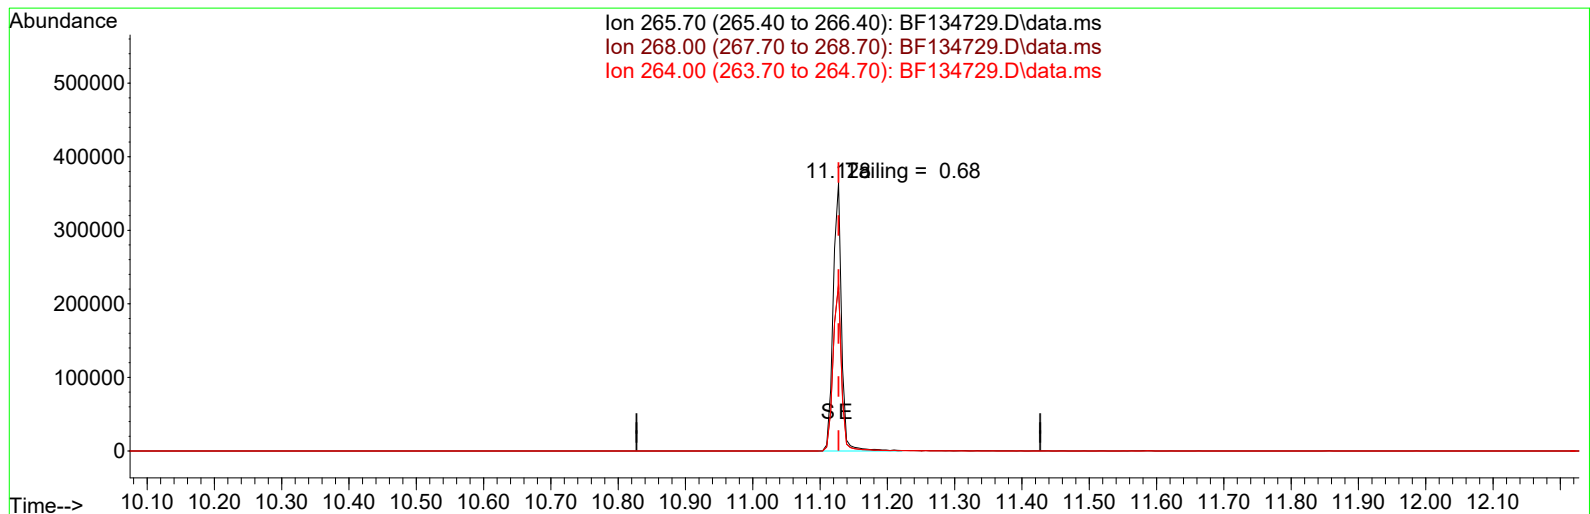

TIC: BF134729.D\data.ms

(70) Pentachlorophenol (C)

11.128min (+ 0.000) 275954.00 ng




response **316016**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	61.71
264.00	59.70	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081123\
Data File : BF134729.D
Acq On : 11 Aug 2023 13:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 12 00:47:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

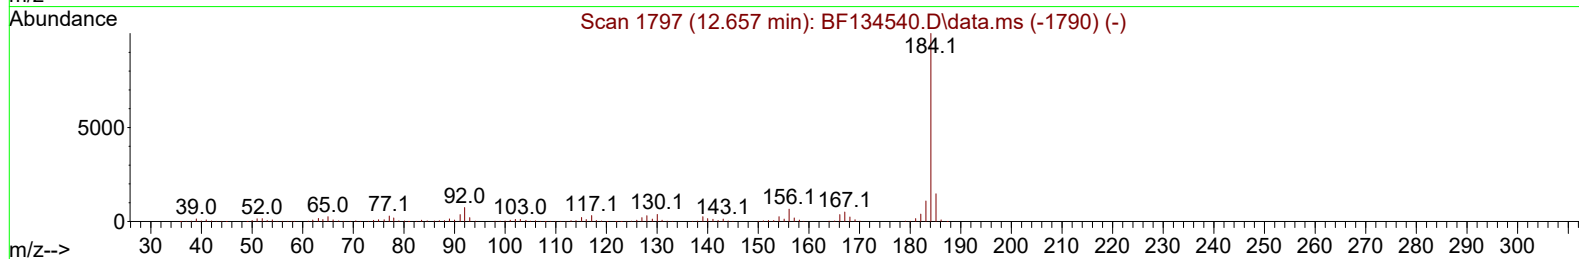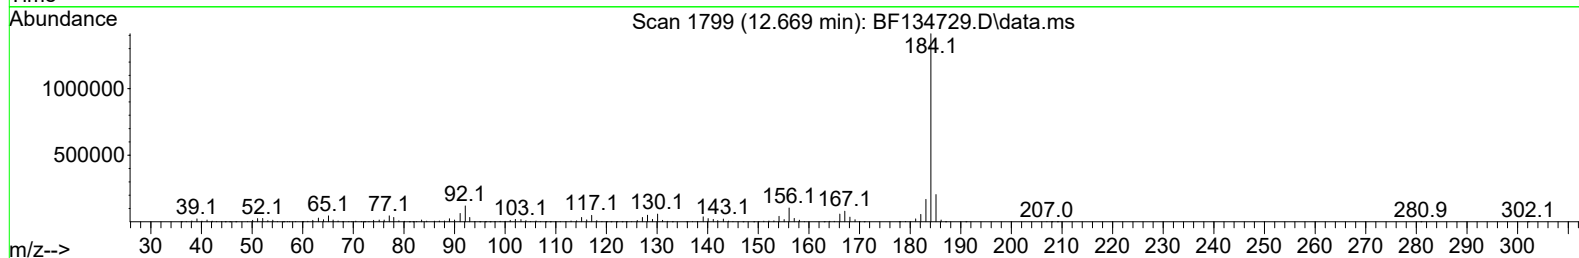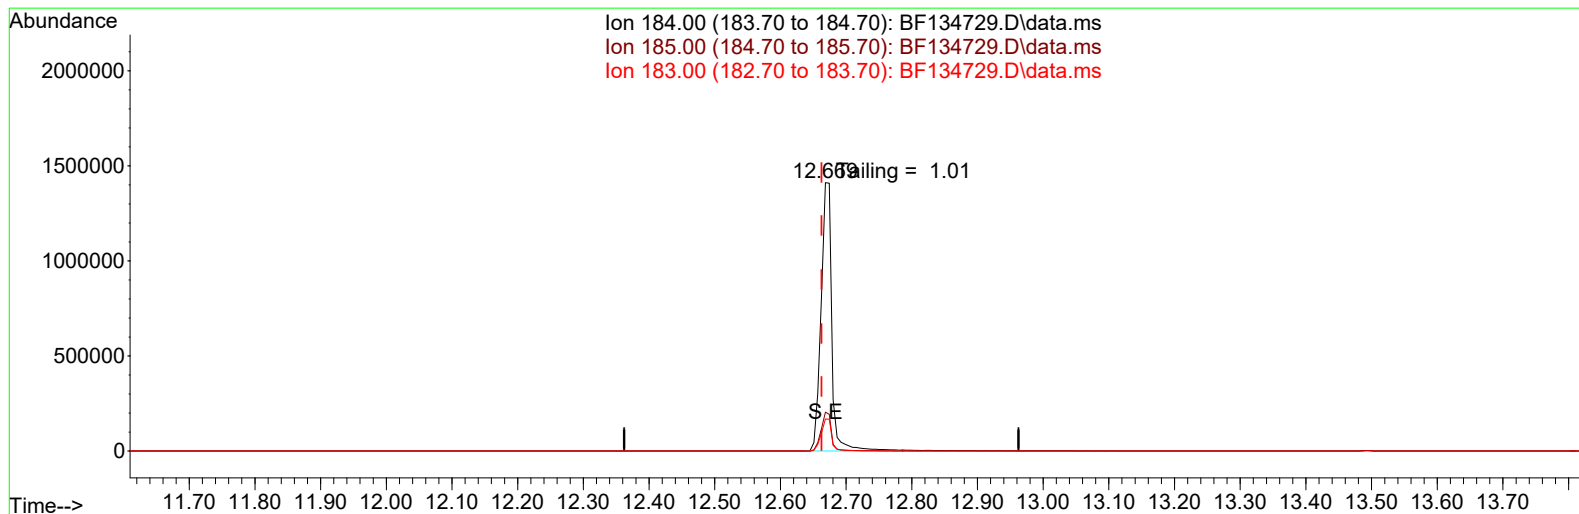

TIC: BF134729.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 681340.74 ng

response 1626951

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.48
183.00	10.80	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/11/2023	BNA_F	<u>BF134729.D</u>
Compound Name	Response	Retention Time
DDT	680703	13.492
DDD	22862	13.192
DDE	996	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23858	704561	3.39

Instrument :
BNA_F
ClientSampleId :
DFTPP