


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081219\
 Data File : BF116181.D
 Acq On : 12 Aug 2019 9:48
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 07 11:13:18 2019

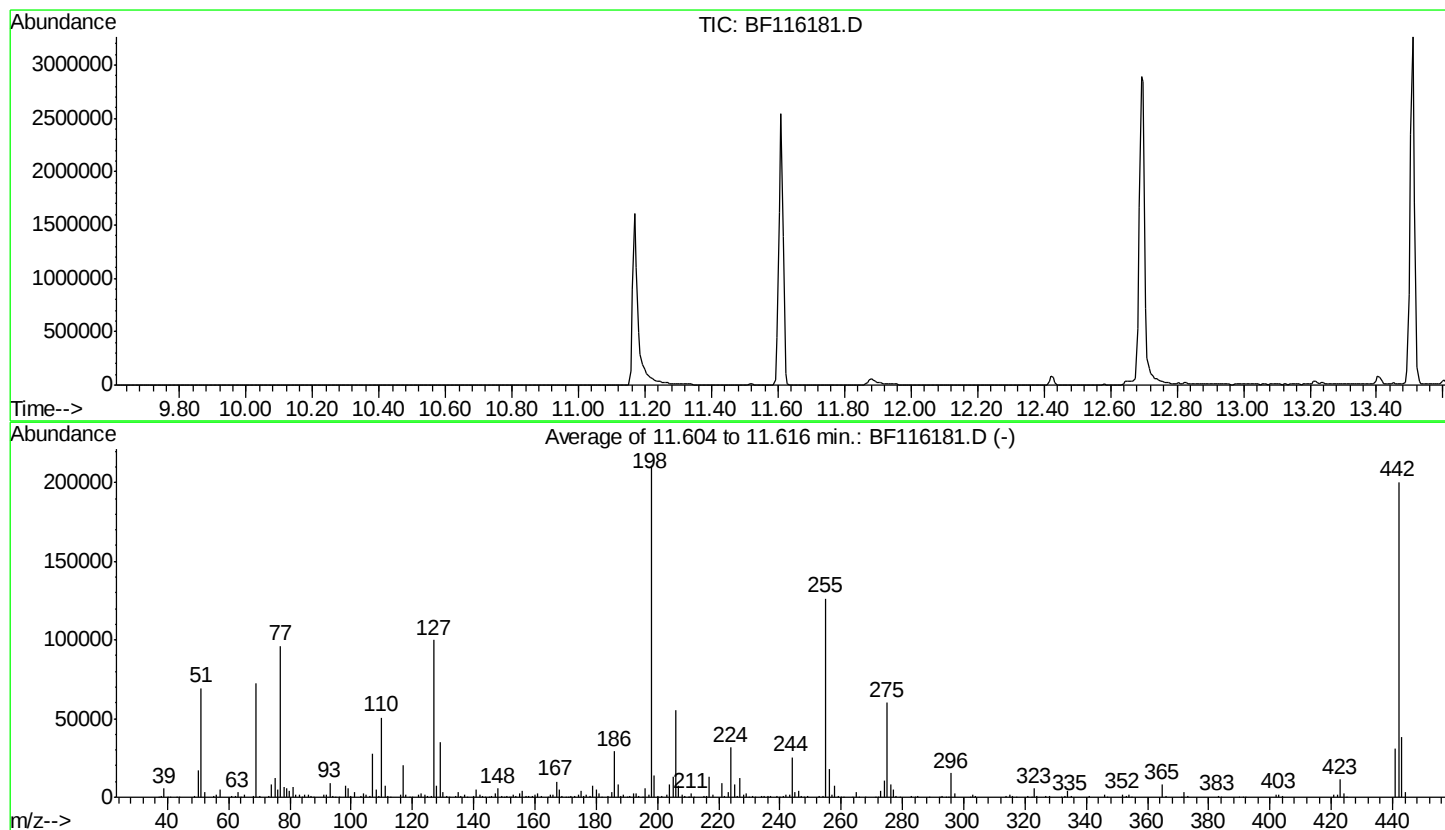

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	69336	PASS
68	69	0.00	2	1.7	1211	PASS
69	198	0.00	100	34.5	72728	PASS
70	69	0.00	2	0.6	450	PASS
127	198	10	80	47.5	100058	PASS
197	198	0.00	2	0.6	1366	PASS
198	198	100	100	100.0	210794	PASS
199	198	5	9	6.8	14245	PASS
275	198	10	60	28.5	60114	PASS
365	198	1	100	3.7	7817	PASS
441	198	0.01	100	14.8	31302	PASS
442	198	50	100	95.1	200512	PASS
443	442	15	24	18.9	37872	PASS